



Automated Measurement and Prediction of Consciousness in Vegetative and Minimally Conscious Patients

Denis Engemann, Federico Raimondo, Jean-Remi King, Mainak Jas, Alexandre Gramfort, Stanislas Dehaene, Lionel Naccache, Jacobo Sitt

► **To cite this version:**

Denis Engemann, Federico Raimondo, Jean-Remi King, Mainak Jas, Alexandre Gramfort, et al.. Automated Measurement and Prediction of Consciousness in Vegetative and Minimally Conscious Patients. ICML Workshop on Statistics, Machine Learning and Neuroscience (Stam-lins 2015), Jul 2015, Lille, France. 2015. <hal-01225254>

HAL Id: hal-01225254

<https://hal.inria.fr/hal-01225254>

Submitted on 26 Nov 2015

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

Automated Measurement and Prediction of Consciousness in Vegetative and Minimally Conscious Patients

Denis A. Engemann*

DENIS.ENGEMANN@GMAIL.COM

Institut du Cerveau et de la Moelle Épineière, ICM, F-75013, Paris, France

Federico Raimondo*

FRAIMONDO@DC.UBA.AR

Laboratorio de Inteligencia Artificial Aplicada, Departamento de Computación FCEyN, UBA, Argentina

Jean-Rémi King

JEANREMI.KING@GMAIL.COM

Institut Mines-Télécom, Télécom ParisTech, CNRS LTCI, France

Mainak Jas

MAINAKJAS@GMAIL.COM

Institut Mines-Télécom, Télécom ParisTech, CNRS LTCI, France

Alex Gramfort

ALEXANDRE.GRAMFORT@TELECOM-PARITECH.FR

Institut Mines-Télécom, Télécom ParisTech, CNRS LTCI, France

Stanislas Dehaene

STANISLAS.DEHAENE@CEA.FR

Cognitive Neuroimaging Unit, Institut National de la Santé et de la Recherche Médicale, U992, F-91191 Gif/Yvett, France

Lionel L. Naccache

LIONEL.NACCACHE@GMAIL.COM

Institut du Cerveau et de la Moelle Épineière, ICM, F-75013, Paris, France

Jacobo D. Sitt

JDSITT@GMAIL.COM

Institut du Cerveau et de la Moelle Épineière, ICM, F-75013, Paris, France

Abstract

Recent findings in clinical neuroscience have emphasized electroencephalography (EEG) as a tool to discriminate different disorders of consciousness (DOC) such as the vegetative and the minimally conscious state. Here we present an automated approach to computing EEG-measures of consciousness and guiding clinical diagnostics of DOC. Our approach capitalizes the automated extraction of statistically validated EEG-measures quantifying biomarkers of consciousness and filing a database thereof. In a second step, statistical models trained on the database of EEG-measures are then used to predict an incoming patient's state of consciousness. For each new patient, the results of the EEG- and the predictions are automatically summarized and deployed to the clinician in form

of a self-contained HTML-report, which supports interactive visualization and navigation. To validate our approach, we replicated previous findings on EEG-measures of consciousness and quantified the robustness of the EEG-measures to loss of temporal and spatial information. Our results suggest that the EEG-measures can be successfully employed in a wide range of practical contexts to measure a patients degree of consciousness.

1. An automated scalable approach to measure and predict consciousness in clinical settings

Advances in contemporary medicine have as consequence that increasingly more patients survive catastrophic brain injuries but remain in disordered consciousness conditions, such as the vegetative (VS) or the minimally conscious state (MCS). Recent brain imaging and neurophysiological studies have enhanced the scientific understanding of these conditions, but have also emphasized novel diag-

nostic challenges (Laureys & Schiff, 2012). The distinction of MCS from VS patients can be elusive even for trained physicians. For example, non-standardized behavioral evaluations can lead to misclassifications of up to 40% (Schnakers et al., 2009), which in turn can lead to erroneous pain-management, prognosis evaluation and even misinformed end-of-life decisions. Furthermore, for a small proportion of patients that are correctly classified as VS (by means of their behavioral responses), functional neuroimaging suggests preserved consciousness (Owen et al., 2006). This poses challenges on multiple, interdisciplinary levels. One such challenge is related to incorporating scientific findings on neural correlates of consciousness into the clinical and diagnostic practice. Over the last decade, abundant electrophysiological signatures of consciousness have been proposed. Recently, a systematic analysis of electroencephalography (EEG) measures has been put forward by Sitt et al. (2014). A set of measures has been identified that allows to differentiate patients in a vegetative state from those in a minimally conscious or conscious state. These measures quantify putative biomarkers of consciousness such as low-frequency brain-rhythms, stimulus-related synchronization of EEG signals (evoked responses), information sharing between electrodes and signal complexity. Importantly, previous multivariate classification analyses suggested that these EEG-measures capture complementary information as they yield superior classification performance when combined. This poses the question of how such advanced analysis of the EEG can be used in practice to facilitate clinical diagnostics.

1.1. A system for guiding clinical diagnostics of consciousness disorders

Here we implemented an automated solution to clinical diagnostics of disorders of consciousness (DOC) based on statistical analysis of clinical EEG. Its goal is to estimate an undiagnosed patient’s degree of consciousness based on the EEG-measures described in Sitt et al. (2014) and to efficiently communicate the EEG-analysis together with the diagnostic prediction. For this purpose we developed a flexible and scalable data analysis workflow that automates processing of EEG recordings, the extraction of EEG-measures and the communication of results (cf. figure 1 for an illustration of the workflow). The solution that we present here is purely based on open source software and is scalable on multiple levels.

For example, by taking advantage of the Python language and its parallel processing libraries such as `joblib`¹, multiple CPU-cores can be used to carry out numerical computations. Previously, the only available option to compute

¹<https://pythonhosted.org/joblib/parallel.html>

the EEG-measures proposed by Sitt et al. (2014) consisted in using local computers and required licenses for commercial software. Moreover, our solution has built-in support for Amazon web services (AWS), which allows to carry out computations in parallel across subjects. With 20 virtual workstations of which each is equipped with 4 CPU-cores for example, the computation time can be cut down by a factor of 80. Currently, for a single recording, all EEG-measures can be computed in about 30 minutes. These benchmarks are particularly relevant for the practical purpose of the system. The current implementation facilitates the computation of reference models that are estimated on EEG-measures from hundreds of clinical recordings to predict unseen patients.

This not only facilitates more frequent updates of these reference models, which may be required for research purposes. It also lowers the maintenance burdens, i.e., of detecting and fixing software bugs. To communicate results efficiently, we devised an HTML-report tool that embeds images together with the requisite Java-script code enabling interactive navigation. This self-contained feature promotes automated dispatch of summary-reports to clinicians or operators, hence, facilitates review and interpretation.

This approach thus minimizes manual interaction or intervention by the operator to produce and review findings and is therefore expected to reduce errors. To the best of our knowledge, this solution is novel and constitutes the first automated workflow for diagnostics of DOC patients. The following sections detail the implementation strategy and present a validation of the proposed solution based on the analysis of clinical EEG data from DOC patients.

1.2. Implementation details

1.2.1. SOFTWARE

Our software solution is based on open source technologies and is written in Python, C, and bash shell scripts. The computation of the EEG-measures described in Sitt et al. (2014) was implemented in Python, taking advantage of the Numpy and Scipy libraries for fast matrix calculus and scientific computing (Jones et al., 2001). Some performance critical computations have been deferred to code written in C, accompanied by Python bindings. Bash scripts are then used to handle distributed computing and distributing jobs using GNU-parallel (Tange, 2011). For general data-processing and visualization the open source software package MNE is used (Gramfort et al., 2013; 2014) The report-technology has meanwhile been made publicly available as part of the MNE package. For unsupervised learning and classification, the scikit-learn library for machine learning is used (Pedregosa et al., 2011).

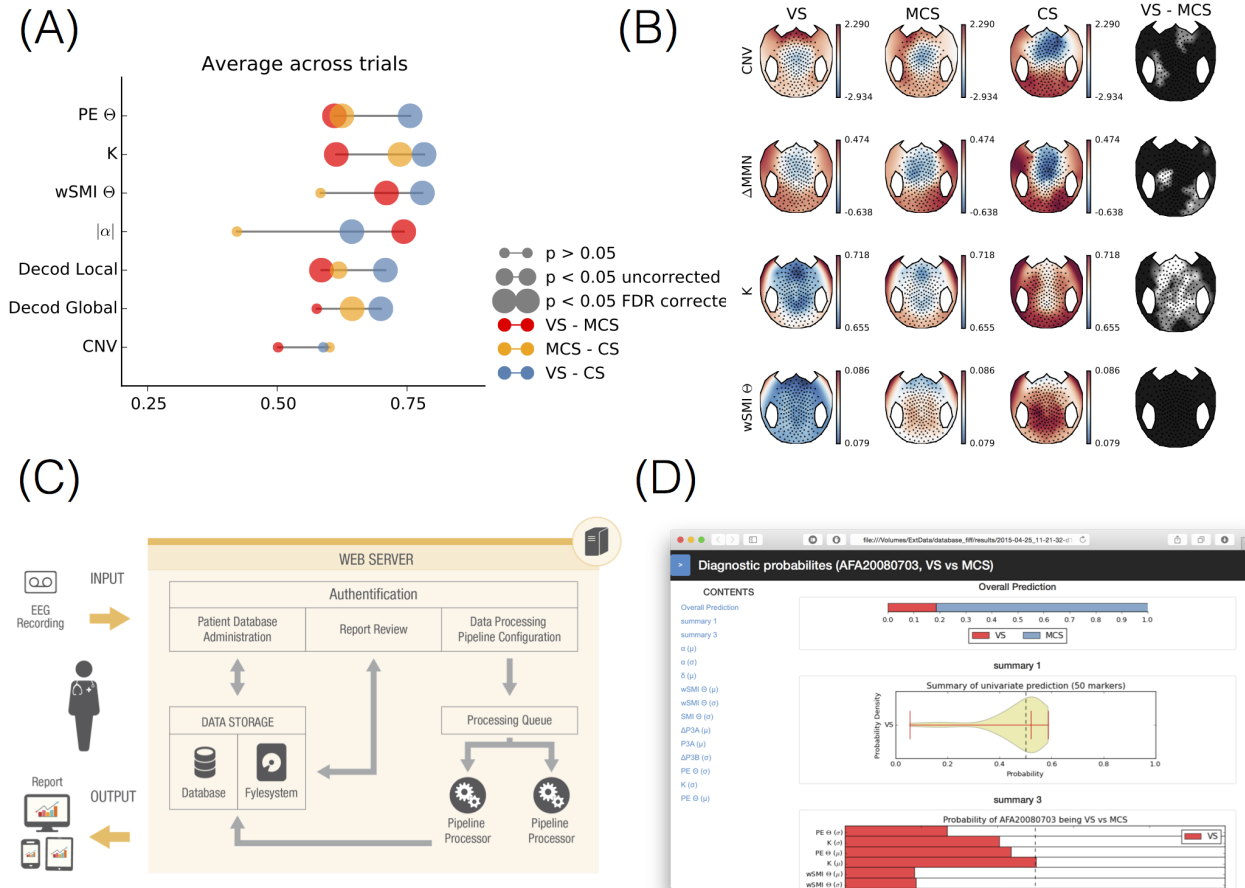


Figure 1. Overview on the automated approach to measurement and diagnostics of consciousness. Panel (A) and (B) illustrate group results for a subset of EEG-measures for different groups of patients suffering from disorders of consciousness (DOC), i.e., vegetative state (VS), minimally conscious state (MCS) and conscious (CS). Panel (A) depicts univariate area under the curve (AUC) scores for mean values across channels. From top to bottom, permutation entropy (PE), complexity measure (K), the wSMI connectivity, normalized alpha-band power, the classification score for the global and the local auditory novelty task, respectively, and the contingent negative variation (CNV). Different colors and different sizes refer to contrasts of interest and significance thresholds, respectively. Big circles refer to false discovery-rate (FDR) corrected p-values. The computation of the EEG-measures was implemented after Sitt et al. (2014), supplementary materials. Panel (B) depicts related topographies for a subset of the measures shown in panel (B). The outermost column shows a non-parametric statistical map based on a Wilcoxon rank sum test, where white, gray and black areas indicate uncorrected p-values greater than 0.05, smaller than 0.05 or smaller than 0.01 respectively. Panel (C) illustrates the overall workflow. EEG data are entered into the system by the operator, the automated pipeline is launched on a web-server, summary reports are dispatched to the operator. Panel (D) shows a screenshot of a diagnostic report that presents the estimated probability of the patient being in a minimally conscious state.

1.2.2. EEG-RECORDINGS AND PROCESSING

For development and validation analyses, the data reported in Sitt et al. (2014) were used. Subjects were stimulated using the auditory *Local-Global* protocol (Bekinschtein et al., 2009). In this protocol, subjects were presented with a series of sounds that contains regularities at two different hierarchical levels, a local level, defined by short-term and a global level, defined by long-term regularities. The deviations from these regularities evoke distinct event-related potentials that are useful to evaluate the cognitive state of the patient. EEG recordings were sampled at 250 Hz with a 256-electrode geodesic sensor net (EGI) referenced to the vertex. Recordings were band-pass filtered (from 0.5 to 45Hz using a 12 order FFT-based Butterfly filter). Data were then epoched from $-200ms$ to $+1336ms$ relative to the onset of the first sound.

The following parameters reflect default settings of our software solution and do not depend on the validation dataset. Trials were excluded based on their amplitude range with a rejection threshold at $100mV$. Trials were subsequently baseline corrected over the first 200 ms window preceding the onset of the first sound. Electrodes with a rejection rate superior to 20% across trials were rejected and were interpolated using a spherical spline interpolation. To remove remaining artifacts, the FastICA (Hyvärinen et al., 2004) algorithm for Independent Component Analysis (ICA) was used in concert with the ADJUST procedure for identifying artefact-related EEG signal components (Mognon et al., 2011). Subsequently, data were re-referenced using an average reference. All data were processed in Python 2.7 using the open source software package MNE (Gramfort et al., 2013; 2014). Figure 2 gives an overview about the single data processing steps.

Note that our EEG-processing workflow is not confined to a specific EEG-vendor and does not require task-related EEG-recordings.

2. Validation of EEG-measures of consciousness

To validate the extraction of the EEG-measures against the reference implementation, we replicated the main analysis from Sitt et al. (2014) on univariate classification (cf. figures 1 and 2, supplement) and we validated the multivariate classification against alternative algorithms and implementations (cf. Figure 3, supplement). We further profiled the EEG-measures by evaluating their discriminative performance as information was removed from the input data. For this purpose, the original data from Sitt et al. (2014) were used. We considered a subset of patient recordings comprising 69 samples of MCS and 76 samples of VS patients. To emulate the impact of different sensor geometry,

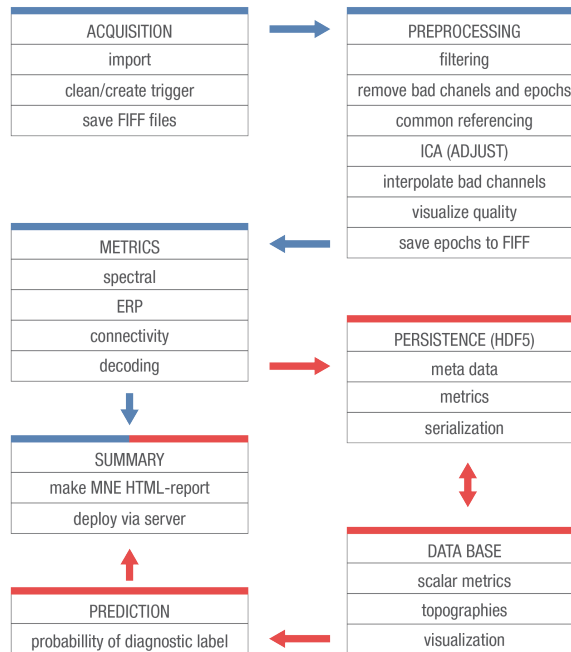


Figure 2. Schematic EEG data-processing workflow. The procedure comprises two complementary routines, depicted by blue and red connecting arrows between the steps. Directly after acquisition, data are converted in to the FIFF file format (cf. Gramfort et al. (2013; 2014)). Subsequently, the EEG data are cleaned from environmental noise, intrinsic and physiological artifacts. This is achieved by peak-to-peak amplitude rejection of contaminated data segments and removal of artifact signal components as estimated by Independent Component Analysis (ICA). Data are then segmented according to task-related events or fixed-length epochs (resting state) and stored to disk. In the next step, relevant EEG-measures are computed and stored to disk together with meta-data and added to the database. Visual summaries of the results are saved into an HTML report. Fed with EEG-measures from the database, a statistical model is employed to estimate the probability of each diagnostic class. Visual summaries of the patient’s measured EEG-measures and the probability estimates are deployed in form of a second HTML report. The entire procedure is scalable and can be executed locally or remotely on multiple workers in a distributed fashion.

the spatial coverage and acquisition settings, the data were spatially (number of sensors) and temporally (sampling frequency) subsampled. Results were then recomputed on the subsampled data and compared to the full data. Classification was based on a support vector machine with an area under the curve (AUC) performance metric. A filter-based feature selection (best k features as defined by univariate F-statistic) and the regularization parameter (C) were tuned using a grid search with 10 fold stratified cross-validation

that was repeated 5 times. Figure 3 depicts measure-wise (average across sensors) central tendencies and dispersion across all subsampled datasets. For details on the computation of the univariate AUC scores, see the supplementary materials.

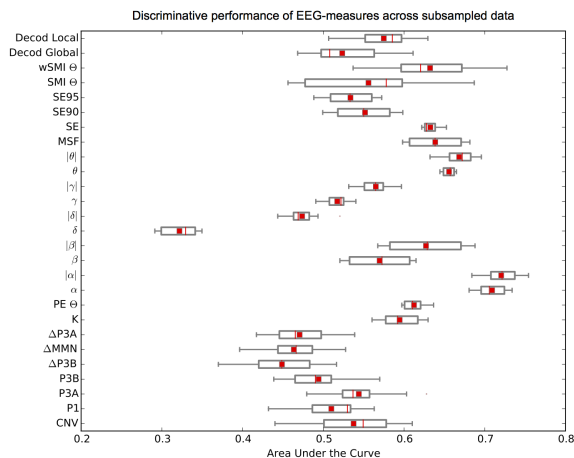


Figure 3. Univariate evaluation of discriminative performance of different EEG-measures as spatial and temporal information is removed from the data. New datasets were derived from temporally and spatially subsampling the original data. To generate a set of realistic electrode nets the original number of electrodes (256) was progressively subdivided by two and remaining electrodes were manually selected. They were chosen such that the resulting electrode net was spatially symmetric and included a subset of standard locations described by the international 10-20 system. In total, 6 electrode nets (256 to 8 electrodes) were compared at 250Hz and 125Hz temporal sampling frequency. The boxplots summarize each EEG-measure individually depicting the central tendency and dispersion of area under the curve (AUC) scores across the datasets. The red lines represent the median, the red squares the mean. The results suggest that certain EEG-measures were more robust across varying density of information in the input data. Note that AUC scores below 0.5 indicate a negative relationship between the respective EEG-measure and the target-category. Acronyms for EEG-measures are explained in the supplementary materials (cf. Table 1). A multivariate comparison is depicted in Figure 4

It can be observed that certain types of measures, for example the wSMI connectivity measure (King et al., 2013) or evoked response measures, such as the contingent negative variation (CNV) exhibit more performance variability across data inputs. In contrast, information theory measures, e.g., PE, K, and low frequency cortical oscillations show little variability, e.g., α , θ and δ . These findings were expected as the connectivity measures naturally benefit from a high spatial sampling density, whereas α power can be computed on single favorably located sensors. This

latter finding extends previously reported results (Sitt et al., 2014). Not only are low-frequency oscillations among the most robust predictors of consciousness, their computation is also highly robust across different sensor configurations and temporal sampling rates. This is of high practical relevance, as it may inform practitioners about reasonable low cost choices for the assessment of consciousness. For instance, the low frequency brain rhythms can be reliably extracted from a few electrodes only using a low temporal sampling frequency. This finding may have practical implications when single measures have to be selected for fast ambulant screening based on low-density EEG. Likewise, these measures remain robust at reduced sampling rates which may be helpful for mobile EEG acquisition setups with limited recording capacity such as for long term recordings.

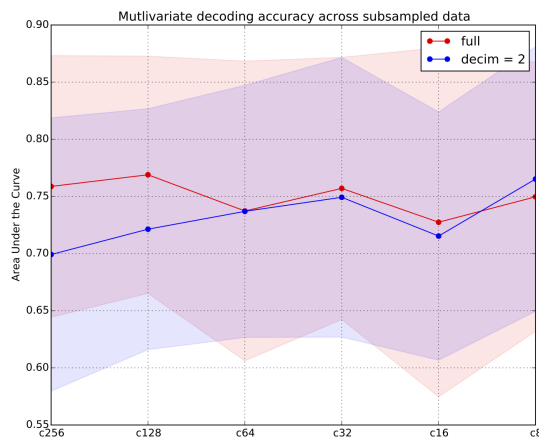


Figure 4. Multivariate evaluation of discriminative performance of different EEG-variables as spatial and temporal information is removed from the data. The points represent cross-validated area under the curve (AUC) scores separately for temporally and spatially subsampled versions of the data. The x-axis depicts different electrode nets, including 256, 128, 64, 32, 16 and 8 electrodes. Lines represent different sampling frequencies, i.e., 250Hz and 125Hz. Areas represent the standard deviation of the AUC score. The overall pattern suggests that spatiotemporal subsampling does not notably affect the classification performance.

Additional insights can be obtained from comparing cross-validated classification performance based on multivariate inputs including all the EEG-measures. Figure 4 depicts such scores for each subsampled version of the input data. The findings show considerable overlapping estimation variance across folds for each dataset, suggesting that for multivariate classification the availability of high-density sampling is not particularly relevant. In other words, regular clinical EEG-setups that commonly include between 32 and 64 channels are sufficient to acquire data

from which reliable EEG-measures can be computed.

To summarize, the experiments provide novel insights regarding the stability, or reliability, of the EEG-measures. The univariate results (cf. Figure 3) highlight certain types of measures that are more robust to loss of information than others. In contrast, the multivariate results (cf. Figure 4) demonstrate that removing temporal and spatial information does not relevantly decrease predictive performance when all information is fed into a statistical model.

3. Conclusion

In the present work we presented an integrated scalable solution for measuring, predicting and guiding clinical diagnostics of disorders of consciousness (DOC). This approach promotes a translation from neuroscience findings and data science technologies to clinical practice. The validation analyses not only suggest a successful implementation of the EEG-measures reported in (Sitt et al., 2014) but also extend our understanding of their practical properties such as their dependency on particular acquisitions setups. Future enhancement in classification and diagnostics are expected from incorporating additional samples (clinical EEG-recordings) and a prediction of the patient's recovery into the proposed solution. Similarly, it should be easily adjustable to other physiological and pathological conditions in which an evaluation of the subject's degree of consciousness is relevant. This would at least include anesthesia and sleep. Our solution, this way, promotes a diagnostic practice emphasizing brain-circuits disorders (Insel & Cuthbert, 2015).

Acknowledgments

References

- Bekinschtein, Tristan A., Dehaene, Stanislas, Rohaut, Benjamin, Tadel, Francois, Cohen, Laurent, and Naccache, Lionel. Neural signature of the conscious processing of auditory regularities. *Proceedings of the National Academy of Sciences*, 2009. doi: 10.1073/pnas.0809667106. URL <http://www.pnas.org/content/early/2009/01/21/0809667106.abstract>.
- Gramfort, A, Luessi, M, Larson, E, Engemann, D A, Strohmeier, D, Brodbeck, C, Goj, R, Jas, M, Brooks, T, Parkkonen, L, and Hämäläinen, M. MEG and EEG data analysis with MNE-Python. *Frontiers in Neuroscience*, 7 (267), 2013. ISSN 1662-453X. doi: 10.3389/fnins.2013.00267.
- Gramfort, A, Luessi, M, Larson, E, Engemann, D, Strohmeier, D, Brodbeck, C, Parkkonen, L, and Hämäläinen, M. MNE software for processing MEG and EEG data. *Neuroimage*, 86(0):446 – 460, 2014. ISSN 1053-8119. doi: <http://dx.doi.org/10.1016/j.neuroimage.2013.10.027>.
- Hyvärinen, Aapo, Karhunen, Juha, and Oja, Erkki. *Independent component analysis*, volume 46. John Wiley & Sons, 2004.
- Insel, Thomas R. and Cuthbert, Bruce N. Brain disorders? precisely. *Science*, 348(6234):499–500, 2015. doi: 10.1126/science.aab2358. URL <http://www.sciencemag.org/content/348/6234/499.short>.
- Jones, Eric, Oliphant, Travis, Peterson, Pearu, et al. SciPy: Open source scientific tools for Python, 2001. URL <http://www.scipy.org/>. [Online; accessed 2015-05-01].
- King, Jean-Rmi, Sitt, JacoboD., Faugeras, Frdric, Rohaut, Benjamin, ElKaroui, Imen, Cohen, Laurent, Naccache, Lionel, and Dehaene, Stanislas. Information sharing in the brain indexes consciousness in noncommunicative patients. *Current Biology*, 23(19):1914 – 1919, 2013. ISSN 0960-9822. doi: <http://dx.doi.org/10.1016/j.cub.2013.07.075>. URL <http://www.sciencedirect.com/science/article/pii/S0960982213009366>.
- Laureys, Steven and Schiff, Nicholas D. Coma and consciousness: paradigms (re) framed by neuroimaging. *Neuroimage*, 61(2):478–491, 2012.
- Mognon, Andrea, Jovicich, Jorge, Bruzzone, Lorenzo, and Buiatti, Marco. Adjust: An automatic eeg artifact detector based on the joint use of spatial and temporal features. *Psychophysiology*, 48(2):229–240, 2011.
- Owen, Adrian M, Coleman, Martin R, Boly, Melanie, Davis, Matthew H, Laureys, Steven, and Pickard, John D. Detecting awareness in the vegetative state. *Science*, 313(5792):1402–1402, 2006.
- Pedregosa, F., Varoquaux, G., Gramfort, A., Michel, V., Thirion, B., Grisel, O., Blondel, M., Prettenhofer, P., Weiss, R., Dubourg, V., Vanderplas, J., Passos, A., Cournapeau, D., Brucher, M., Perrot, M., and Duchesnay, E. Scikit-learn: Machine learning in Python. *Journal of Machine Learning Research*, 12:2825–2830, 2011.
- Schnakers, Caroline, Vanhauzenhuyse, Audrey, Giacino, Joseph, Ventura, Manfredi, Boly, Melanie, Majerus, Steve, Moonen, Gustave, and Laureys, Steven. Diagnostic accuracy of the vegetative and minimally conscious state: clinical consensus versus standardized neurobehavioral assessment. *BMC neurology*, 9(1):35, 2009.

Sitt, J D, King, J-R, El Karoui, I, Rohaut, B, Faugeras, F, Gramfort, A, Cohen, L, Sigman, M, Dehaene, S, and Naccache, L. Large scale screening of neural signatures of consciousness in patients in a vegetative or minimally conscious state. *Brain*, 137(8):2258–2270, 2014.

Tange, O. Gnu parallel - the command-line power tool. ;login: *The USENIX Magazine*, 36(1):42–47, Feb 2011.
URL <http://www.gnu.org/s/parallel>.