

Digital Twins in Critical Care: What, When, How, Where, Why?

J. Geoffrey Chase*, Cong Zhou*, Jennifer L. Knopp*, Geoffrey M. Shaw**, Katharina Näswall***, Jennifer HK Wong***, Sanna Malinen****, Knut Moeller*, Balazs Benyo⁶*, Yeong, Shiong Chiew⁷*, Thomas Desai⁸*

*Univ of Canterbury, Dept of Mechanical Eng, Christchurch, NZ (email: Geoff.Chase@canterbury.ac.nz)

**Christchurch Hospital, Dept of Intensive Care, Christchurch, NZ (email: Geoff.Shaw@cdhb.health.nz)

***Univ of Canterbury, School of Psychology, Speech and Hearing Christchurch, NZ (email:

jennifer.wong@canterbury.ac.nz)

****Univ of Canterbury, School of Business, Christchurch, NZ (email: sanna.malinen@canterbury.ac.nz)

5* Furtwangen University, Inst for Technical Medicine, V-S, Germany (knut.moeller@hs-furtwangen.de)

6* Budapest Univ of Technology, Dept of Information Science, Budapest, Hungary (bbenyo@iit.bme.hu)

7* Monash University Malaysia, Kuala Lumpur, Malaysia (chiew.yeong.shiong@monash.edu)

8* Liege University, GIGA In-Silico Medicine, Liege, Belgium (tdesaive@uliege.be)

Abstract: Healthcare and intensive care unit (ICU) medicine in particular, are facing a devastating tsunami of rising demand multiplied by increasing chronic disease and aging demographics, which is unmatched by society's ability to pay. Digital technologies and automation have brought significant productivity gains to many industries, and manufacturing in particular, but not yet to medicine. In manufacturing, digital twins, model-based optimisation of manufacturing systems and equipment, are a rapidly growing means of further enhancing productivity and quality. This concept intersects well with the model-based decision support and control just beginning to emerge into clinical use, offering the opportunity to personalise care, and improve its quality and productivity. This article presents digital twins in a manufacturing concept and translates it into clinical practice, and then reviews the state of the art in key areas of ICU medicine.

Copyright © 2021 The Authors. This is an open access article under the CC BY-NC-ND license (<https://creativecommons.org/licenses/by-nc-nd/4.0/>)

Keywords: Digital Twins, ICU, Critical Care, Physiological Modeling, Virtual Patient, Virtual Cohort.

1. INTRODUCTION

Intensive care unit (ICU) patients are very complex and highly variable, making management difficult. Aging demographics, chronic disease, and increasing life spans are driving increasing cost and reducing equity of access to care (Baumol et al., 2012, Dombovy, 2002, Halpern, 2009, Halpern, 2011, Orsini et al., 2014, Shorr, 2002, Truog et al., 2006, van Exel et al., 2015). There is thus a significant need to improve productivity and quality of care.

Personalised care using patient-specific models identified from clinical data offers the means to directly manage intra- and inter- patient (Chase et al., 2018b) variability. It adds automation to care, using digital technologies to improve quality and cost, as in many other sectors, but much less in medicine (Baumol et al., 2012, Economist, 2011, Mickelthwait, 2011). Thus, some level of automation will be necessary given society's increasing inability to meet rising costs and provide equal equity of access to care (OECD, 2015).

Hyper-automation and digital twins (DT) capture the essence of this model-based approach and are a major growth area in manufacturing (Cimino et al., 2019, Panetta, 2019). Reduced cost and optimisation arise from using sensor data to monitor, model, and manage real-world systems. In medicine, the difference is the humans in the loop, patient and clinicians.

This review translates digital twin definitions into the medical application space. It focuses on the models and methods required for hyper-automation, especially the impact of the

humans in the loop in cyber-physical-human systems who are not as integral in the manufacturing case. Finally, this state of the art review explores the key technical and innovation uptake issues required to successfully bring DTs into medical care.

2. DIGITAL TWINS AND VIRTUAL PATIENTS

2.1 Digital Twin Definition

Digital twins have risen at the intersection of Industry 4.0 and the internet of things (IoT) relying on converging technologies in big data, sensors, and cloud computing. A DT is “a virtual copy of a system able to interact with the physical system in a bi-directional way” (Cimino et al., 2019, Kritzinger et al., 2018). They are cyber-physical-systems. The bi-directional exchange of information synchronizes virtual system response to match the physical system to “forecast and optimise the behavior of the physical system in real time”.

In manufacturing digital twins sit on top of a “control layer” of supporting technologies, under a top layer of “enterprise resource planning” which integrates organizational functions and goals into the use of the DT. This DT organisation is simplified and shown schematically in Fig. 1. In Fig. 1 both upper and lower layers inform the DT and its design / use. The DT itself is connected through the control layer to its physical counterpart in real-time and uses modeling and computation to continually update the virtual twin (Negri et al., 2017).

DTs are defined by their integration (Kritzinger et al., 2018). A digital model (DM) has no interaction with the physical system. A digital shadow (DS) is updated with data from the

physical system, but does not inform its control. A DT arises when physical system data is used to update the DM, and the resulting simulation is used to control the physical system. To date, there are few true DTs in use (Cimino et al., 2019).

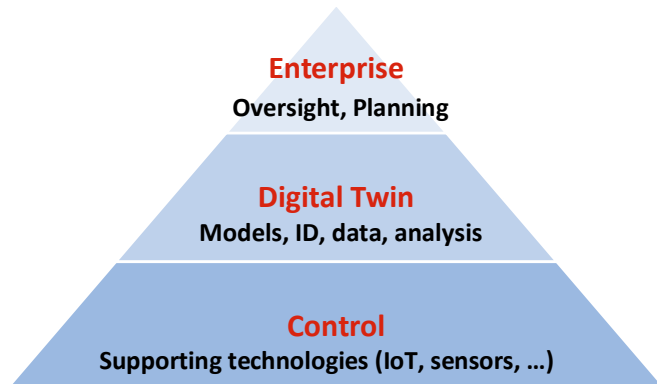


Figure 1: DT structure between supporting technologies (IoT, sensors, communications) and an enterprise layer integrating DT use into meeting organizational goals (overall protocols, oversight, and planning), based on (Chen, 2005).

2.2 Digital Twins in Medicine

In medicine, the physical system is the patient, or a particular organ or physiological system to be managed. A human is also in the loop clinically, particularly in the enterprise layer (Fig. 1) where protocolised use of a DT is designed, integrated, and managed in care (Chase et al., 2016, Chase et al., 2018b). Within the framework of Fig. 1 a DT in medicine would fit in a control loop in Fig. 2, where bi-directional information to and from the DT is clear in the loop. The modeling and DT update process is illustrated in Fig. 3, where the incoming data in Fig. 2 can be used to update the model at any time to provide accurate prediction in response to proposed interventions.

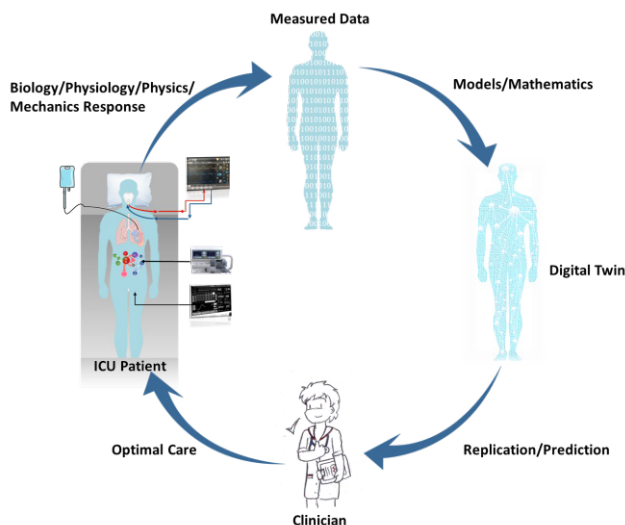


Figure 2: DT control loop in medicine with clinical staff in the control loop.

How interventions are optimised in a medical DT is based on a protocol to optimise patient care, by clinical staff at the “enterprise” level in Fig. 1. Finally, it is important to note the clinician in the loop in Fig. 2 is there for safety, but can be fully removed in full automation.

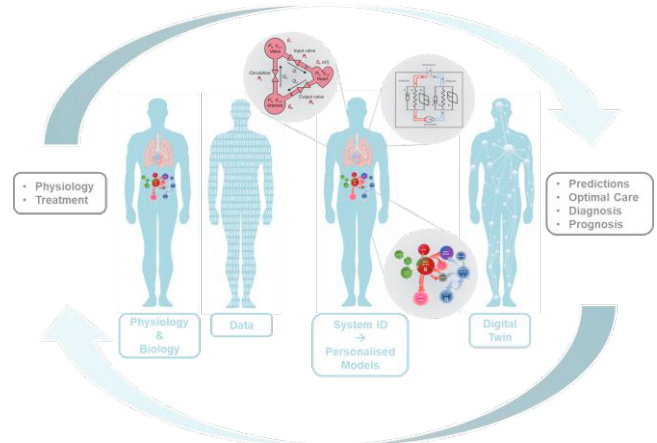


Figure 3: DT model creation and updating from clinical data.

2.3 Virtual Patients (Digital Twin Models and Methods)

Medicine and physiology offer many DMs, models informed by data, but not receiving real-time patient data (Hunter et al., 2010, Nickerson et al., 2016, Safaei et al., 2016, Viceconti et al., 2016). However, most are too complex to be personalized in real-time with available data (Chase et al., 2018b).

DS models are increasingly common, able to be personalised, and are differentiated by their identifiability from relatively limited clinical data in many cases (Chase et al., 2011b, Chase et al., 2019, Desai et al., 2019, Morton et al., 2019b). They have been used to assess new medical technology applications (Zhou et al., 2018, Zhou et al., 2019) and protocols (Fisk et al., 2012, Uyttendaele et al., 2018). However, very few are used in regular care, and thus are not DTs, where < 1% of model-based decision support systems are implemented beyond testing, let alone standard care (Garg et al., 2005, Wears et al., 2005).

Finally, a virtual patient (VP) is a DS, DM, or DT model able to be identified from relevant bedside data, and providing accurate prediction validation in response to modeled inputs (Fig. 4). A collection of VPs creates a virtual cohort (VC) where VPs created from retrospective data can be grouped into a VC for developing and optimizing new protocols. A VP model suitable for being a digital twin should be validated in the ability to accurately predict patient-specific outcomes to specific interventions, as well as accurately capturing cohort response in simulating a new protocol over a unit, where the first enables the DT and the second allows the protocol to be optimised for the “enterprise layer” in Fig. 1 and is based on clinical goals (Chase et al., 2018a, Chase et al., 2018b).

2.4 Application of DTs in ICU Medicine

There are 3-4 core areas of ICU medicine: glycemic control (GC); cardiovascular (CVS) care; sedation delivery (SD); and mechanical ventilation (MV). They affect 30-80% of all ICU patient and suffer variability in care and outcomes due to lack of physiological insight from the data available leading to difficulty in managing inter- and intra- patient variability. Moreover, they have significant negative impact from both over or under delivering of care, and are a leading cause of ICU admission, length of stay, cost, and/or mortality. Thus, each core area could gain significant advantage from a DT providing a far clearer physiological picture of patient state

from the data available (Chase et al., 2018b). In each area, virtual patient models exist at levels ranging from DM to DT in their integration with the patient (Figs. 1-2) and into care.

GC is the most advanced area. There are multiple metabolic system models based on decades of research (Chase et al., 2011a, Chase et al., 2018b). However, relatively few have achieved patient level validation (Hovorka et al., 2008, Le Compte et al., 2009, Lin et al., 2011, Van Herpe et al., 2006, Wilinska et al., 2008). GC protocols have been optimised using these models (Blaha et al., 2016, Evans et al., 2012, Fisk et al., 2012, Knopp et al., 2019, Le Compte et al., 2011, Lonergan et al., 2006, Mesotten et al., 2017, Pielmeier et al., 2010, Van Herpe et al., 2013, Wilinska et al., 2008). However, very few have delivered clinical results very close to those simulated before implementation (Chase et al., 2007, Fisk et al., 2012, Knopp et al., 2019, Wilinska et al., 2011). Similarly, at the cohort level, validation has only been presented for one model in multiple ICU capacities, including cross validation from randomised trial data (Chase et al., 2007, Chase et al., 2010, Dickson et al., 2018, Fisk et al., 2012).

MV virtual patient models are much less advanced, as only two models accurately capture predict lung mechanics evolution with changing ventilator settings (Morton et al., 2019a, Morton et al., 2020, Zhou et al., 2021). In particular, critical metrics, such as recruitment volume retained as pressures change, peak volume and pressures, lung elastances, and work of breathing. These metrics offer more accurate insight not previously available to optimise MV, where MV doubles the cost per day (Dasta et al., 2005). They are currently entering first clinical trials (Kim et al., 2020b), and have been tested in neonatal cohorts (Kim et al., 2019, Kim et al., 2020a).

Finally, for SD only fundamental models have been developed with no virtual patient or cohort validation (Rudge et al., 2006). Similarly, CVS has developed models to estimate key parameters for clinically managing circulation and cardiac stroke volume (Murphy et al., 2020a, Murphy et al., 2020b, Pironet et al., 2015, Smith et al., 2020a, Smith et al., 2020b, Smith et al., 2021). Both areas have foundation elements for a DM, but have not progressed to DT solutions at this time.

2.5 What is Missing?

The only bi-directional DTs in clinical ICU use are in GC, and they are not fully automated with a human in the loop (Knopp et al., 2019, Stewart et al., 2016). Thus, the main element missing is technological and not model or control based. Specifically, there is a need to create greater interoperability and access to data from the range of ventilators and infusion pumps in the ICU, which has been a great source of difficulty due to proprietary and other reasons (Hudson et al., 2018, Jaleel et al., 2020, Mavrogiorgou et al., 2019).

3. INNOVATION UPTAKE

Having all the technologies, models, and protocols to create DTs for use as standard of care is not enough. The “*enterprise layer*” of Fig. 1 also includes decision making on adoption of new standards of care. Adoption is a decision made at both the ICU and clinician level, as well as higher management and/or a health system level.

Alarming, patients are reported to benefit from only 30-50% of the validated healthcare technologies (Grol, 2001, Schuster et al., 2005), indicating at least half of healthcare innovations fail to be successfully adopted, even after being clinically validated in earlier development stages.

We consider *technology adoption* to be the acceptance, integration, and use of new technology in an environment. This requires consideration of factors at the individual, the team/unit, and the organisational system levels.

3.1 Factors Impacting Technology Adoption

Majority of research on technology adoption focuses on factors relating to individual employees, including employees' past experience with technology (Gagnon et al., 2012, Koivunen et al., 2018, McGinn et al., 2011, Schreiweis et al., 2019), perceptions of the new technology's usability, the expected benefits of the innovation (system usefulness; Kruse et al., 2016), and ease of use (Gagnon et al., 2012). The cognitive processes from learning how to use the technology (Koivunen et al., 2018), motivation to use the technology (McGinn et al., 2011), and trusting the technology (Lluch, 2011) also drive technology adoption decisions.

Furthermore, emotion-based factors can similarly hinder the adoption process, such as fear of technology (e.g., changes at work, Koivunen and Saranto, 2018; Kruse et al., 2016; fear of depersonalization of healthcare, Lluch, 2011; fear of being replaced by technology, undermined credibility, impact on professional identity, Koivunen and Saranto, 2018; fear of reduced quality of care, Gagnon et al., 2012; Koivunen and Saranto, 2018; McGinn et al., 2011) and disinterest towards the technology (Koivunen et al., 2018). Importantly, the capacity to provide high-standard quality of care is a core value in healthcare professionals (Ko et al., 2018) and thereby the introduction of new technology may give rise to fear of reduced quality of care.

While individual factors are crucial to consider in advancing adoption, the hierarchical nature of healthcare must also be considered. Healthcare delivery teams rely on conformity through hierarchical decision-making processes to maintain performance and minimise risk (Hughes et al., 2016). The power dynamics likely influence the process of technology adoption, as hierarchy within teams can hinder communication and collaboration (Baker et al., 2011) and reduce opportunities for peer support in the adoption process. Furthermore, colleagues' negative attitudes resisting technology is a known barrier, particularly so when the resistance comes from an influential peer (Gagnon et al., 2012, Greenhalgh et al., 2010, Greenhalgh et al., 2017, van Deen et al., 2019).

3.2 A Way Forward

Successful technology adoption requires an approach that considers the individual, team, and system factors that can influence uptake. This includes previous history with technology, perceptions and emotions towards technology, how technology impacts the delivery of quality of care, and the hierarchical structure and power dynamics of the healthcare delivery sector. At the organizational system-level, communications about and support for technology use from

healthcare management is crucial for sustainable uptake (Gagnon et al., 2012, Ingebrigtsen et al., 2014, Kruse et al., 2016, Schreiweis et al., 2019).

The extensive research greatly contributes to the knowledge and understanding of the technology adoption problem, although mainly from an individual employee's perspective. Indeed, *the problem still exists*. There is a further need to address the socio-relational aspects of the system, particularly those centered on the decision-makers who enable technology adoption and uptake.

5. CONCLUSION

ICU medical care needs dramatic productivity improvements to ensure better care, meet dramatically growing demand, and provide continuing equity of access. This review shows there are a few DTs already in use, and the foundation elements for significant growth in the nearer future. However, there is a strong need to address both the technology of interoperability and the social science of innovation uptake to ensure these solutions reach their potential impact in transforming care.

REFERENCES

- Baker, L., Egan-Lee, E., Martimianakis, M. A. and Reeves, S. 2011. Relationships of power: implications for interprofessional education. *Journal of interprofessional care*, 25, 98-104.
- Baumol, W. J. and De Ferranti, D. M. 2012. *The cost disease : why computers get cheaper and health care doesn't*, New Haven, Yale University Press.
- Blaha, J., Barteczko-Grajek, B., Berezowicz, P., Charvat, J., Chvojka, J., Grau, T., Holmgren, J., Jaschinski, U., Kopecky, P., Manak, J., Moehl, M., Paddle, J., Pasculli, M., Petersson, J., Petros, S., Radrizzani, D., Singh, V. and Starkopf, J. 2016. Space GlucoseControl system for blood glucose control in intensive care patients—a European multicentre observational study. *BMC Anesthesiol*, 16, 8.
- Chase, J., Desaive, T. and Preiser, J. C. 2016. Virtual Patients and Virtual Cohorts: A New Way to Think About the Design and Implementation of Personalized ICU Treatments. In: VINCENT, J. L. (ed.) *Annual Update in Intensive Care and Emergency Medicine*.
- Chase, J. G., Shaw, G. M., Lotz, T., Lecompte, A., Wong, J., Lin, J., Loneragan, T., Willacy, M. and Hann, C. E. 2007. Model-based insulin and nutrition administration for tight glycaemic control in critical care. *Curr Drug Deliv*, 4, 283-96.
- Chase, J. G., Suhaimi, F., Penning, S., Preiser, J. C., Le Compte, A. J., Lin, J., Pretty, C. G., Shaw, G. M., Moorhead, K. T. and Desaive, T. 2010. Validation of a model-based virtual trials method for tight glycemic control in intensive care. *Biomed Eng Online*, 9, 84.
- Chase, J. G., Le Compte, A. J., Suhaimi, F., Shaw, G. M., Lynn, A., Lin, J., Pretty, C. G., Razak, N., Parente, J. D. and Hann, C. E. 2011a. Tight glycemic control in critical care-The leading role of insulin sensitivity and patient variability: A review and model-based analysis. *Computer Methods and Programs in Biomedicine*, 102, 156-171.
- Chase, J. G., Le Compte, A. J., Preiser, J. C., Shaw, G. M., Penning, S. and Desaive, T. 2011b. Physiological modeling, tight glycemic control, and the ICU clinician: what are models and how can they affect practice? *Ann Intensive Care*, 1, 11.
- Chase, J. G., Desaive, T., Bohe, J., Cnop, M., De Block, C., Gunst, J., Hovorka, R., Kalfon, P., Krinsley, J., Renard, E. and Preiser, J. C. 2018a. Improving glycemic control in critically ill patients: personalized care to mimic the endocrine pancreas. *Crit Care*, 22, 182.
- Chase, J. G., Preiser, J. C., Dickson, J. L., Pironet, A., Chiew, Y. S., Pretty, C. G., Shaw, G. M., Benyo, B., Moeller, K., Safaei, S., Tawhai, M., Hunter, P. and Desaive, T. 2018b. Next-generation, personalised, model-based critical care medicine: a state-of-the-art review of in silico virtual patient models, methods, and cohorts, and how to validation them. *Biomed Eng Online*, 17, 24.
- Chase, J. G., Benyo, B. and Desaive, T. 2019. Glycemic control in the intensive care unit: A control systems perspective. *Annual Reviews in Control*, 48, 359-368.
- Chen, D. 2005. Enterprise-control system integration—an international standard. *International journal of production research*, 43, 4335-4357.
- Cimino, C., Negri, E. and Fumagalli, L. 2019. Review of digital twin applications in manufacturing. *Computers in Industry*, 113, 103130.
- Dasta, J. F., McLaughlin, T. P., Mody, S. H. and Piech, C. T. 2005. Daily cost of an intensive care unit day: The contribution of mechanical ventilation. *Crit Care Med*, 33, 1266-1271.
- Desaive, T., Horikawa, O., Ortiz, J. P. and Chase, J. G. 2019. Model-based management of cardiovascular failure: Where medicine and control systems converge. *Annual Reviews in Control*.
- Dickson, J. L., Stewart, K. W., Pretty, C. G., Flechet, M., Desaive, T., Penning, S., Lambermont, B. C., Benyo, B., Shaw, G. M. and Chase, J. G. 2018. Generalisability of a Virtual Trials Method for Glycaemic Control in Intensive Care. *IEEE Trans Biomed Eng*, 65, 1543-1553.
- Dombovy, M. L. 2002. U.S. health care in conflict--Part I. The challenges of balancing cost, quality and access. *Physician Exec*, 28, 43-7.
- Economist, T. 2011. Patient, heal thyself. *The Economist* London, UK: The Economist.
- Evans, A., Le Compte, A., Tan, C. S., Ward, L., Steel, J., Pretty, C. G., Penning, S., Suhaimi, F., Shaw, G. M. and Desaive, T. 2012. Stochastic Targeted (STAR) Glycemic Control: Design, Safety, and Performance. *Journal of Diabetes Science and Technology*, 6, 102-115.
- Fisk, L., Lecompte, A., Penning, S., Desaive, T., Shaw, G. and Chase, J. G. 2012. STAR Development and Protocol Comparison. *IEEE Trans Biomed Eng*, 59, 3357-3364.
- Gagnon, M.-P., Desmartis, M., Labrecque, M., Car, J., Pagliari, C., Pluye, P., Frémont, P., Gagnon, J., Tremblay, N. and Légaré, F. 2012. Systematic review of factors influencing the adoption of information and communication technologies by healthcare professionals. *Journal of medical systems*, 36, 241-277.
- Garg, A. X., Adhikari, N. K., McDonald, H., Rosas-Arellano, M. P., Devereaux, P. J., Beyene, J., Sam, J. and Haynes, R. B. 2005. Effects of computerized clinical decision support systems on practitioner performance and patient outcomes: a systematic review. *JAMA*, 293, 1223-38.
- Greenhalgh, T. and Stones, R. 2010. Theorising big IT programmes in healthcare: strong structuration theory meets actor-network theory. *Social science & medicine*, 70, 1285-1294.
- Greenhalgh, T., Wherton, J., Papoutsis, C., Lynch, J., Hughes, G., Hinder, S., Fahy, N., Procter, R. and Shaw, S. 2017. Beyond adoption: a new framework for theorizing and evaluating

- nonadoption, abandonment, and challenges to the scale-up, spread, and sustainability of health and care technologies. *Journal of medical Internet research*, 19, e367.
- Grol, R. 2001. Successes and failures in the implementation of evidence-based guidelines for clinical practice. *Med Care*, 39, 1146-54.
- Halpern, N. A. 2009. Can the costs of critical care be controlled? *Curr Opin Crit Care*, 15, 591-6.
- Halpern, S. D. 2011. ICU capacity strain and the quality and allocation of critical care. *Curr Opin Crit Care*, 17, 648-57.
- Hovorka, R., Chassin, L. J., Ellmerer, M., Plank, J. and Wilinska, M. E. 2008. A simulation model of glucose regulation in the critically ill. *Physiol Meas*, 29, 959-78.
- Hudson, F. and Clark, C. 2018. Wearables and medical interoperability: the evolving frontier. *Computer*, 51, 86-90.
- Hughes, A. M., Gregory, M. E., Joseph, D. L., Sonesh, S. C., Marlow, S. L., Lacerenza, C. N., Benishek, L. E., King, H. B. and Salas, E. 2016. Saving Lives: A Meta-Analysis of Team Training in Healthcare. *Journal of applied psychology*, 101, 1266-1304.
- Hunter, P., Coveney, P. V., De Bono, B., Diaz, V., Fenner, J., Frangi, A. F., Harris, P., Hose, R., Kohl, P., Lawford, P., McCormack, K., Mendes, M., Omholt, S., Quarteroni, A., Skar, J., Tegner, J., Randall Thomas, S., Tollis, I., Tsamardinos, I., Van Beek, J. H. and Viceconti, M. 2010. A vision and strategy for the virtual physiological human in 2010 and beyond. *Philos Transact A Math Phys Eng Sci*, 368, 2595-614.
- Ingebrigtsen, T., Georgiou, A., Clay-Williams, R., Magrabi, F., Hordern, A., Prgomet, M., Li, J., Westbrook, J. and Braithwaite, J. 2014. The impact of clinical leadership on health information technology adoption: systematic review. *International journal of medical informatics*, 83, 393-405.
- Jaleel, A., Mahmood, T., Hassan, M. A., Bano, G. and Khurshid, S. K. 2020. Towards medical data interoperability through collaboration of healthcare devices. *IEEE Access*, 8, 132302-132319.
- Kim, K. T., Knopp, J., Dixon, B. and Chase, G. 2019. Quantifying neonatal pulmonary mechanics in mechanical ventilation. *Biomedical Signal Processing and Control*, 52, 206-217.
- Kim, K. T., Knopp, J., Dixon, B. and Chase, J. G. 2020a. Mechanically ventilated premature babies have sex differences in specific elastance: A pilot study. *Pediatric Pulmonology*, 55, 177-184.
- Kim, K. T., Morton, S., Howe, S., Chiew, Y. S., Knopp, J. L., Docherty, P., Pretty, C., Desaive, T., Benyo, B. and Szlavetz, A. 2020b. Model-based PEEP titration versus standard practice in mechanical ventilation: a randomised controlled trial. *Trials*, 21, 130.
- Knopp, J. L., Lynn, A. M., Shaw, G. M. and Chase, J. G. 2019. Safe and effective glycaemic control in premature infants: observational clinical results from the computerised STAR-GRYPHON protocol. *Arch Dis Child Fetal Neonatal Ed*, 104, F205-F211.
- Ko, M., Wagner, L. and Spetz, J. 2018. Nursing home implementation of health information technology: Review of the literature finds inadequate investment in preparation, infrastructure, and training. *INQUIRY: The Journal of Health Care Organization, Provision, and Financing*, 55, 0046958018778902.
- Koivunen, M. and Saranto, K. 2018. Nursing professionals' experiences of the facilitators and barriers to the use of telehealth applications: a systematic review of qualitative studies. *Scandinavian journal of caring sciences*, 32, 24-44.
- Kritzinger, W., Karner, M., Traar, G., Henjes, J. and Sihm, W. 2018. Digital Twin in manufacturing: A categorical literature review and classification. *IFAC-PapersOnLine*, 51, 1016-1022.
- Kruse, C. S., Kristof, C., Jones, B., Mitchell, E. and Martinez, A. 2016. Barriers to electronic health record adoption: a systematic literature review. *Journal of medical systems*, 40, 1-7.
- Le Compte, A., Chase, J., Lynn, A., Hann, C., Shaw, G., Wong, X. and Lin, J. 2009. Blood Glucose Controller for Neonatal Intensive Care: Virtual trials development and 1st clinical trials. *Journal of Diabetes Science and Technology (JoDST)*, 3, 1066-1081.
- Le Compte, A. J., Chase, J. G., Lynn, A., Hann, C. E., Shaw, G. M. and Lin, J. 2011. Development of blood glucose control for extremely premature infants. *Comput Methods Programs Biomed*, 102, 181-91.
- Lin, J., Razak, N. N., Pretty, C. G., Le Compte, A., Docherty, P., Parente, J. D., Shaw, G. M., Hann, C. E. and Geoffrey Chase, J. 2011. A physiological Intensive Control Insulin-Nutrition-Glucose (ICING) model validated in critically ill patients. *Comput Methods Programs Biomed*, 102, 192-205.
- Lluch, M. 2011. Healthcare professionals' organisational barriers to health information technologies—A literature review. *International journal of medical informatics*, 80, 849-862.
- Lonergan, T., Lecompte, A., Willacy, M., Chase, J. G., Shaw, G. M., Wong, X. W., Lotz, T., Lin, J. and Hann, C. E. 2006. A Simple Insulin-Nutrition Protocol for Tight Glycemic Control in Critical Illness: Development and Protocol Comparison. *Diabetes Technol Ther*, 8, 191-206.
- Mavrogiorgou, A., Kiourtis, A., Perakis, K., Pitsios, S. and Kyriazis, D. 2019. IoT in healthcare: achieving interoperability of high-quality data acquired by IoT medical devices. *Sensors*, 19, 1978.
- Meginn, C. A., Grenier, S., Duplantie, J., Shaw, N., Sicotte, C., Mathieu, L., Leduc, Y., Légaré, F. and Gagnon, M.-P. 2011. Comparison of user groups' perspectives of barriers and facilitators to implementing electronic health records: a systematic review. *BMC medicine*, 9, 1-10.
- Mesotten, D., Dubois, J., Van Herpe, T., Van Hooijdonk, R. T., Wouters, R., Coart, D., Wouters, P., Van Assche, A., Veraghtert, G., De Moor, B., Wauters, J., Wilmer, A., Schultz, M. J. and Van Den Berghe, G. 2017. Software-guided versus nurse-directed blood glucose control in critically ill patients: the LOGIC-2 multicenter randomized controlled clinical trial. *Crit Care*, 21, 212.
- Micklethwait, J. 2011. Taming Leviathan. *The Economist*. London, UK: The Economist.
- Morton, S. E., Knopp, J. L., Chase, J. G., Möller, K., Docherty, P., Shaw, G. M. and Tawhai, M. 2019a. Predictive virtual patient modelling of mechanical ventilation: impact of recruitment function. *Annals of biomedical engineering*, 47, 1626-1641.
- Morton, S. E., Knopp, J. L., Chase, J. G., Docherty, P., Howe, S. L., Möller, K., Shaw, G. M. and Tawhai, M. 2019b. Optimising mechanical ventilation through model-based methods and automation. *Annual Reviews in Control*.
- Morton, S. E., Knopp, J. L., Tawhai, M. H., Docherty, P., Heines, S. J., Bergmans, D. C., Möller, K. and Chase, J. G. 2020. Prediction of Lung Mechanics Throughout Recruitment Maneuvers in Pressure-Controlled Ventilation. *Computer Methods and Programs in Biomedicine*, 105696.
- Murphy, L., Davidson, S., Chase, J. G., Knopp, J. L., Zhou, T. and Desaive, T. 2020a. Patient-Specific Monitoring and Trend

- Analysis of Model-Based Markers of Fluid Responsiveness in Sepsis: A Proof-of-Concept Animal Study. *Annals of biomedical engineering*, 48, 682-694.
- Murphy, L., Chase, J., Davidson, S., Smith, R. and Desaive, T. Minimally Invasive Model Based Stressed Blood Volume as an Index of Fluid Responsiveness. In: HIRCHE, S., ed. Proceedings 21st IFAC World Congress, IFAC Papers-Online, 2020b Berlin, Germany. Elsevier, 6-pages.
- Negri, E., Fumagalli, L. and Macchi, M. 2017. A review of the roles of digital twin in CPS-based production systems. *Procedia Manufacturing*, 11, 939-948.
- Nickerson, D., Atalag, K., De Bono, B., Geiger, J., Goble, C., Hollmann, S., Lonien, J., Muller, W., Regierer, B., Stanford, N. J., Golebiewski, M. and Hunter, P. 2016. The Human Physiome: how standards, software and innovative service infrastructures are providing the building blocks to make it achievable. *Interface Focus*, 6, 20150103.
- Oecd 2015. FOCUS on Health Spending @ OECD Health Statistics 2015. *OECD Health Statistics 2015*, July 2015, 1-8.
- Orsini, J., Blaak, C., Yeh, A., Fonseca, X., Helm, T., Butala, A. and Morante, J. 2014. Triage of Patients Consulted for ICU Admission During Times of ICU-Bed Shortage. *J Clin Med Res*, 6, 463-8.
- Panetta, K. 2019. Hyperautomation, blockchain, AI security, distributed cloud and autonomous things drive disruption and create opportunities in this year's strategic technology trends. *Smarter with Gartner*. [Accessed 27 April 2020].
- Pielmeier, U., Andreassen, S., Juliussen, B., Chase, J. G., Nielsen, B. S. and Haure, P. 2010. The Glucosafe system for tight glycemic control in critical care: a pilot evaluation study. *J Crit Care*, 25, 97-104.
- Pironet, A., Desaive, T., Geoffrey Chase, J., Morimont, P. and Dauby, P. C. 2015. Model-based computation of total stressed blood volume from a preload manoeuvre. *Math Biosci*, 265, 28-39.
- Rudge, A., Chase, J., Shaw, G. and Lee, D. 2006. Physiological modelling of agitation-sedation dynamics including endogenous agitation reduction. *Medical Engineering & Physics*, 28, 629-638.
- Safaei, S., Bradley, C. P., Suresh, V., Mithraratne, K., Muller, A., Ho, H., Ladd, D., Hellevik, L. R., Omholt, S. W., Chase, J. G., Muller, L. O., Watanabe, S. M., Blanco, P. J., De Bono, B. and Hunter, P. J. 2016. Roadmap for cardiovascular circulation model. *J Physiol*.
- Schreiweis, B., Pobiruchin, M., Strotbaum, V., Suleder, J., Wiesner, M. and Bergh, B. 2019. Barriers and facilitators to the implementation of ehealth services: systematic literature analysis. *Journal of medical Internet research*, 21, e14197.
- Schuster, M. A., McGlynn, E. A. and Brook, R. H. 2005. How Good Is the Quality of Health Care in the United States? *The Milbank quarterly*, 83, 843-895.
- Shorr, A. F. 2002. An update on cost-effectiveness analysis in critical care. *Curr Opin Crit Care*, 8, 337-43.
- Smith, R., Balmer, J., Pretty, C. G., Mehta-Wilson, T., Desaive, T., Shaw, G. M. and Chase, J. G. 2020a. Incorporating pulse wave velocity into model-based pulse contour analysis method for estimation of cardiac stroke volume. *Computer Methods and Programs in Biomedicine*, 105553.
- Smith, R., Balmer, J., Pretty, C., Shaw, G. and Chase, J. Clinical application of a model-based cardiac stroke volume estimation method. In: HIRCHE, S., ed. Proceedings 21st IFAC World Congress, IFAC Papers-Online, 2020b Berlin, Germany. 6-pages.
- Smith, R., Murphy, L., Pretty, C. G., Desaive, T., Shaw, G. M. and Chase, J. G. 2021. Tube-load model: A clinically applicable pulse contour analysis method for estimation of cardiac stroke volume. *Computer Methods and Programs in Biomedicine*, 204, 10-pages.
- Stewart, K. W., Pretty, C. G., Tomlinson, H., Thomas, F. L., Homlok, J., Noemi, S. N., Illyes, A., Shaw, G. M., Benyo, B. and Chase, J. G. 2016. Safety, efficacy and clinical generalization of the STAR protocol: a retrospective analysis. *Ann Intensive Care*, 6, 24.
- Truog, R. D., Brock, D. W., Cook, D. J., Danis, M., Luce, J. M., Rubenfeld, G. D., Levy, M. M., Task Force on Values, E. and Rationing in Critical, C. 2006. Rationing in the intensive care unit. *Crit Care Med*, 34, 958-63; quiz 971.
- Uyttendaele, V., Knopp, J. L., Piroette, M., Guiot, J., Morimont, P., Lambermont, B., Shaw, G. M., Desaive, T. and Chase, J. G. 2018. Preliminary results from the STAR-Liège clinical trial: Virtual trials, safety, performance, and compliance analysis. *IFAC-PapersOnLine*, 51, 355-360.
- Van Deen, W. K., Cho, E. S., Pustolski, K., Wixon, D., Lamb, S., Valente, T. W. and Menchine, M. 2019. Involving end-users in the design of an audit and feedback intervention in the emergency department setting—a mixed methods study. *BMC health services research*, 19, 1-13.
- Van Exel, J., Baker, R., Mason, H., Donaldson, C., Brouwer, W. and Eurova, Q. T. 2015. Public views on principles for health care priority setting: findings of a European cross-country study using Q methodology. *Soc Sci Med*, 126, 128-37.
- Van Herpe, T., Espinoza, M., Pluymers, B., Goethals, I., Wouters, P., Van Den Berghe, G. and De Moor, B. 2006. An adaptive input-output modeling approach for predicting the glycemia of critically ill patients. *Physiol Meas*, 27, 1057-69.
- Van Herpe, T., Mesotten, D., Wouters, P. J., Herbots, J., Voets, E., Buyens, J., De Moor, B. and Van Den Berghe, G. 2013. LOGIC-Insulin Algorithm-Guided Versus Nurse-Directed Blood Glucose Control During Critical Illness: The LOGIC-1 single-center randomized, controlled clinical trial. *Diabetes Care*, 36, 189-194.
- Viceconti, M. and Hunter, P. 2016. The Virtual Physiological Human: Ten Years After. *Annu Rev Biomed Eng*, 18, 103-23.
- Wears, R. L. and Berg, M. 2005. Computer technology and clinical work: still waiting for Godot. *JAMA*, 293, 1261-3.
- Wilinska, M. E., Chassin, L. and Hovorka, R. 2008. In Silico Testing—Impact on the Progress of the Closed Loop Insulin Infusion for Critically Ill Patients Project. *Journal of Diabetes Science and Technology*, 2, 417-423.
- Wilinska, M. E., Blaha, J., Chassin, L. J., Cordingley, J. J., Dormand, N. C., Ellmerer, M., Haluzik, M., Plank, J., Vlasselaers, D., Wouters, P. J. and Hovorka, R. 2011. Evaluating glycemic control algorithms by computer simulations. *Diabetes Technol Ther*, 13, 713-22.
- Zhou, C., Chase, J. G., Knopp, J., Sun, Q., Tawhai, M., Möller, K., Heines, S. J., Bergmans, D. C., Shaw, G. M. and Desaive, T. 2021. Virtual patients for mechanical ventilation in the intensive care unit. *Computer Methods and Programs in Biomedicine*, 199, Paper #105912, 24-pages.
- Zhou, T., Dickson, J. L., Shaw, G. M. and Chase, J. G. 2018. Continuous Glucose Monitoring Measures Can Be Used for Glycemic Control in the ICU: An In-Silico Study. *J Diabetes Sci Technol*, 12, 7-19.
- Zhou, T., Knopp, J. L. and Chase, J. G. 2019. The state of variability: A vision for descriptors of glycaemia. *Annual Reviews in Control*, 48, 472-484.