

A New Tissue-Engineered Product Indicated For Bone Reconstruction: A Proof-Of-Concept

Randy Buzisa Mbuku^{*1,2}, Christelle Sanchez^{*3}, Robin Evrard^{1,2}, Alexandre Englebert^{1,2}, Julie Manon^{1,2}, Valentin Henriot⁴, Gregory Nolens⁴, Khanh Tran Duy⁵, Thomas Schubert², Yves Henrotin^{3,6,7}, Olivier Cornu^{1,2}

Presenting Author: Yves Henrotin, yhenrotin@uliege.be

¹Neuro Musculo SKEletal lab, IREC, UCLouvain, Brussels, Belgium

²Orthopedic Surgery and trauma Department, Cliniques Universitaires Saint-Luc, Brussels, Belgium

³MusculoSKEletal Innovative research Lab, University of Liège, Center for Interdisciplinary Research on Medicines, Liège, Belgium

⁴Cerhum SA, Liège, Belgium

⁵3D-SIDE SA, Mont-Saint-Guibert, Belgium

⁶Physical Therapy and Rehabilitation department, Princess Paola Hospital, Vivalia, Marche-en-Famenne, Belgium

⁷Artialis SA, Liège, Belgium

* These authors share first authorship

Abstract text (max 300 words plus References and Acknowledgements)

Objectives

To design slow resorption patient-specific bone graft whose properties of bone regeneration are increased by its geometry and composition and to assess it in in-vitro and in-vivo models.

Materials and methods

A graft composed by hydroxyapatite (HA) and β -TCP was designed as a cylinder with 3D gyroid porosities and 7 mm medullary space based on swine's anatomy. It was produced using a stereolithography 3D-printing machine (V6000, Prodways).

Sterile bone grafts impregnated with or without a 10 μ g/mL porcine BMP-2 (pBMP-2) solution were implanted into porcine femurs in a bone loss model. Bone defect was bi-weekly evaluated by X-ray during 3 months. After sacrifice, microscanner and non-decalcified histology analysis were conducted on biopsies. Finally, osteoblasts were cultured inside the bone graft or in monolayer underneath the bone graft. Cell viability, proliferation, and gene expression were assessed after 7 and 14 days of cell culture (n=3 patients).

Results


3D scaffolds were successfully manufactured with a composition of 80% HA and 20% β -TCP $\pm$ 5% with indentation compressive strength of 4.14 MPa and bending strength of 11.8MPa.

In vivo study showed that bone regeneration was highly improved in presence of pBMP-2. Micro-CT shows a filling of the gyroid sinuses of the implant (*Figure 1*).

In vitro, the presence of BMP2 did not influence the viability of the osteoblasts and the mortality remained below 3%. After 7 days, the presence of BMP2 in the scaffold significantly increased by 85 and 65% the COL1A1 expression and by 8 and 33-fold the TNAP expression by osteoblasts in the monolayer or in the scaffold, respectively. This BMP2 effect was transient in monolayer and did not modify gene expression at day 14.

Conclusion

BMP2-impregnated bone graft is a promising patient-personalized 3D-printed solution for bone defect regeneration, by promoting neighboring host cells recruitment and solid new bone formation.

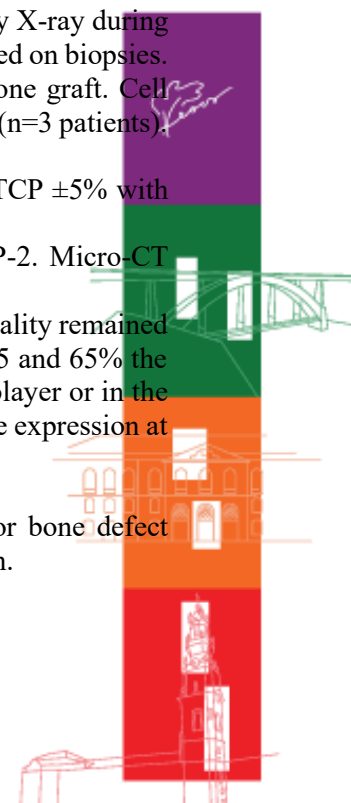

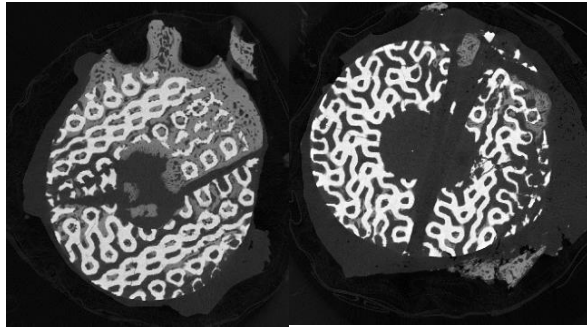


Figure 1 . 12-week Coronal micro-CT section with of the ceramic implant impregnated (left) or not (right) with BMP-2 porcine.
Good filling of the scaffold is observed in the presence of BMP-2

Name and e-mail address of author for correspondence: Randy Buzisa Mbuku, randy.buzisambuku@uclouvain.be

Abstract Category/Topic (select from the table): Tissue Engineering and Regenerative

Free keywords (up to 4): Bone, biomaterials, personalized, regeneration

Selected type of communication (Oral or Poster): Oral

