

Review Article

Challenges for Biomarker Discovery in Body Fluids Using SELDI-TOF-MS

Muriel De Bock,¹ Dominique de Seny,² Marie-Alice Meuwis,³ Jean-Paul Chapelle,¹ Edouard Louis,⁴ Michel Malaise,² Marie-Paule Merville,¹ and Marianne Fillet¹

¹Laboratory of Clinical Chemistry, GIGA Research, University of Liège, CHU, B36, 4000 Liège 1, Belgium

²Department of Rheumatology, GIGA Research, University of Liège, CHU, B36, 4000 Liège 1, Belgium

³Proteomic Platform, GIGA Research, University of Liège, CHU, B36, 4000 Liège 1, Belgium

⁴Department of Hepato-Gastroenterology, GIGA Research, University of Liège, CHU, B36, 4000 Liège 1, Belgium

Correspondence should be addressed to Marianne Fillet, marianne.fillet@ulg.ac.be

Received 27 June 2009; Accepted 1 September 2009

Academic Editor: Pieter C. Dorrestein

Copyright © 2010 Muriel De Bock et al. This is an open access article distributed under the Creative Commons Attribution License, which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.

Protein profiling using SELDI-TOF-MS has gained over the past few years an increasing interest in the field of biomarker discovery. The technology presents great potential if some parameters, such as sample handling, SELDI settings, and data analysis, are strictly controlled. Practical considerations to set up a robust and sensitive strategy for biomarker discovery are presented. This paper also reviews biological fluids generally available including a description of their peculiar properties and the preanalytical challenges inherent to sample collection and storage. Finally, some new insights for biomarker identification and validation challenges are provided.

1. Introduction

The objective of biomarker discovery is to identify specific protein markers susceptible to improve early diagnosis survey therapeutic outcomes and facilitate the development of novel drug candidates [1, 2]. The methodology relies on differential protein expression profiling. The fundamental approach is based on the assumption that the pathology of concern will affect some physiological processes causing changes in the protein expression levels. Proteins generating similar signals in both sample groups are ignored while significantly up- and downregulated proteins become potential biomarkers. Differential expression profiling requires both a sensitive technology to discern any tiny differences and a high-throughput system in order to process large series of samples required to reach statistical significance. Protein differential display techniques such as two-dimensional gel electrophoresis (2-DE), one- or two-dimensional liquid chromatographic (LC-MS), or surface-enhanced laser desorption/ionization time of flight mass spectrometry (SELDI-TOF-MS) are regarded as the most powerful tools for establishing fingerprint profiles [3–6].

Many reports regarding the application of the SELDI-TOF-MS technology have been published since its introduction in 1993 [7] and its first use for disease detection [8]. One of the key features of SELDI-TOF-MS is its ability to provide rapid protein expression profiles from a variety of biological samples with minimal requirements for purification and separation of proteins prior to mass spectrometry. SELDI-TOF-MS profiling studies revealed that biological fluids contain many proteins with low molecular weight (<15 kDa) not resolved on conventional 2D gels [6, 9].

As can be seen in Figure 1, the SELDI technique consists in surface arrays involving various chromatographic models based on both classic chemistries (normal phase, hydrophobic, cation- and anion-exchange surfaces) and specifically affinity-coated surfaces (immobilized metal affinity capture : IMAC). After the binding phase of the sample to these surfaces, the unbound proteins are washed out while retained molecules are overlaid with an energy-absorbing matrix. In the final step, mass spectra are recorded using a laser for the ionization and a TOF mass spectrometer for its resolving power.

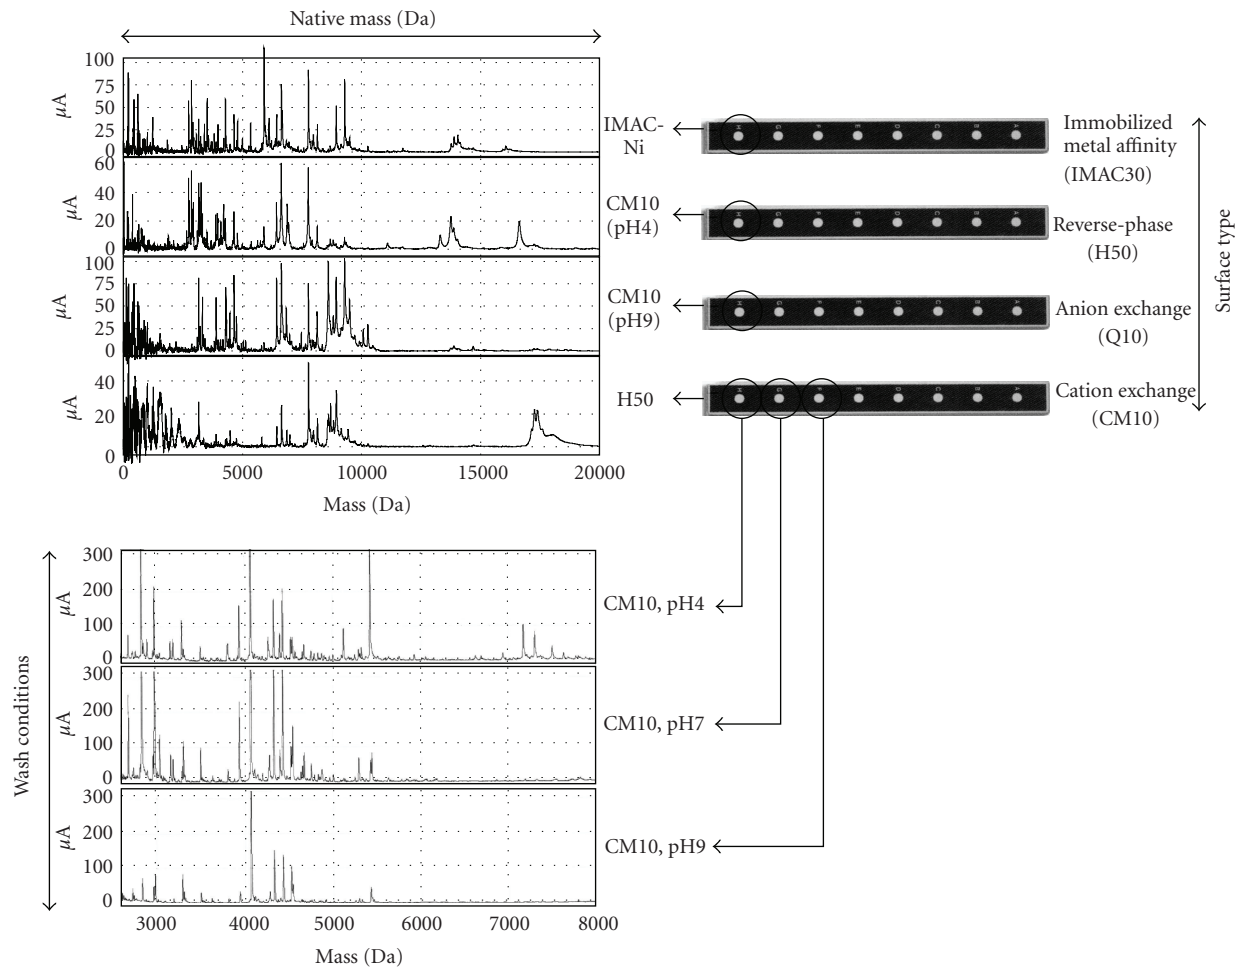


FIGURE 1: Effects of different ProteinChip array surfaces and wash conditions. The combination of ProteinChip array surface types and wash conditions maximize the potential for protein biomarker discovery.

Recent interest in the field has yielded a large number of candidate biomarkers in various diseases [10–35]. However, the small size and poor design of some studies drove validation of these biomarkers quite challenging [36–41].

In the context of clinical proteomic using SELDI-TOF-MS, many recent reviews discussed newly identified disease biomarkers [13, 21, 22, 24, 27, 30, 35, 42–44]. The present review focuses on technical challenges encountered with the SELDI-TOF-MS technology taking into account new insights coming from the last three years. Critical steps that should be undertaken to avoid any bias, to maximize reproducibility and detection sensitivity, with the final aim to find relevant, specific, and robust biomarkers are addressed [45, 46]. For prospective studies, current knowledge on the different biological fluid sources available for SELDI-TOF-MS experiments is described presenting their respective advantages and limitations.

2. Study Design

A successful biomarker research program starts with a careful study design and the preparation of a detailed

protocol. Many manuscripts report encountered problems, emphasizing the importance of Standard Operating Procedures (SOPs), clinical protocols, instrument tuning, and stabilization [37–40, 47–63]. Only critical points will be discussed in this review.

In the early phase of biomarker discovery, the clinical question addressed has to be defined in the disease(s) context collecting adequate control samples. Indeed, it can be criticized that in many published studies, patients were compared to healthy subjects rather than to patients presenting similar diseases or clinical signs.

Experimental workflow and technologies have to be selected with great care. The avoidance of bias is not trivial and must be addressed throughout the whole study, from its design to the data analysis and interpretation (cf. Figure 2). Current proteomics and genomics technologies are extremely sensitive and can detect very small changes in expression levels. Some of these changes may arise from biological differences related to disease or pharmacological treatment. They could also result from the heterogeneity of the patient panels tested across multiples sites, the inherent biological complexity, and the diversity of sample

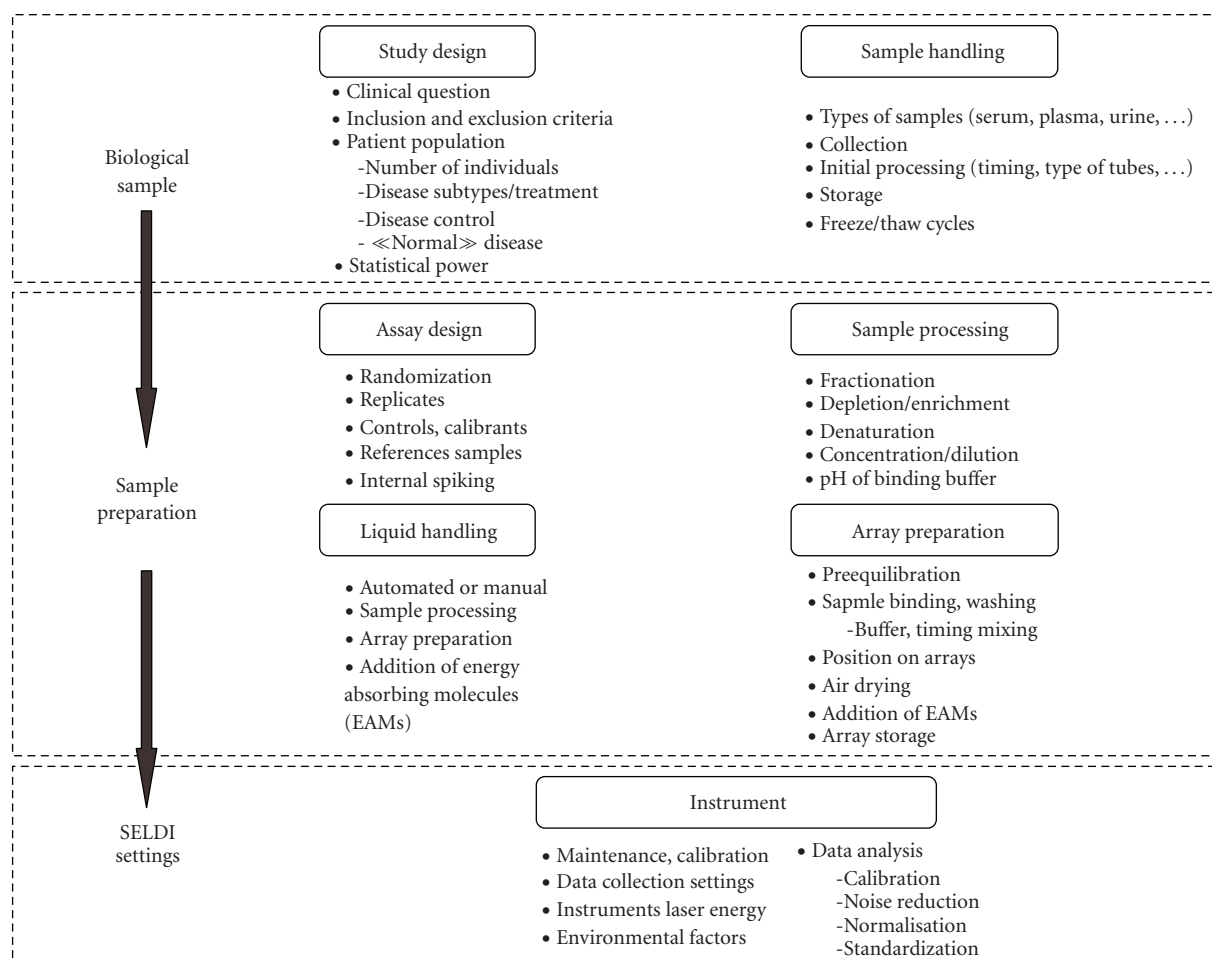


FIGURE 2: Experimental variables that can affect proteomics data. Most of the steps shown are involved in all proteomics workflows, but SELDI technology performs many of them on a single platform.

types. Small differences in sample collection, processing, and analytical techniques could have some impact on the outcomes of the study. As a consequence, clinical data may be site-, study-, population-, or sample-dependent, without any actual clinical relevance [53, 62, 64–66]. The key factor for maximizing reproducibility in biomarker research is to identify and minimize all potential sources of preanalytical and analytical bias [53, 55] (Table 1). Adherence to strict guidelines and SOPs is critical to reach the highest operating standards for data quality and reproducibility [37, 38, 47, 50, 51, 53, 55, 62, 63, 67]. SOPs also facilitate the validation of biomarkers by other groups using different sets of samples.

3. Sample Handling and Preparation

Besides the instrumentation and the methodologies related to chromatography-mass spectrometry analysis, the nature, quality, and number of clinical samples to process are key elements to be considered for any proteomic approaches.

3.1. Selection of Body Fluid. In order to provide positive answer to any precise clinical question, the investigator has to make a choice among the most relevant biological target samples (body fluid, tissue, etc.). Many criteria must be considered at this level, that is, availability, easiness of collection, stability, composition, proximity with disease location, patient discomfort, ethics, and so forth.

For biomarker discovery using SELDI-TOF-MS, a great variety of biological sample types can be used; major applications concern biofluids (plasma, serum, urine, saliva, cerebrospinal liquid, bronchoalveolar wash out, nipple aspirate fluid, tears, amniotic fluid) [1, 10–14, 18, 19, 21, 22, 24, 28, 42, 48, 49, 68–77], and tissues or cell extracts [78, 79]. Among them, serum, plasma, urine, and saliva are the most popular. Many variables related to collection, storage, and conditions for sample preparations have to be carefully considered. These parameters have been commented in literature according to the nature of the biofluids [48, 49, 54, 57, 61, 67, 73, 74, 80–84]. In this section of the review, consensus opinions derived from these recent studies are provided. Advantages and drawbacks of the most popular

TABLE 1: Factors that impact preanalytical and analytical bias.

Preanalytical bias	
<i>Patients information</i>	Age, gender, ethnicity
	Disease subtype and/or severity
	Medical background
	Health background
	Smoking status, alcohol intake, diet, other risk factors
	Drug treatments
	Patient position (seated/standing/lying), daily moment of collection
	Type of control (healthy or disease)
	Location of sample collection (single or multisite)
<i>Sample characteristics</i>	Study inclusion and exclusion criteria
	Number of individuals
	Type (blood, serum, plasma, urine, cerebrospinal fluid, cell lysate, etc.)
<i>Sample-handling procedures</i>	Source (banked or prospectively collected)
	Collection protocols (initial processing, procedure, timing, type of anticoagulant, type of tubes, number of sites, etc.)
<i>Analytical bias</i>	Storage procedures (time, aliquoting, storage materials, temperature, freeze-thaw cycles, etc.)
<i>Sample-Processing procedures</i>	Fractionation and depletion methods
	Processing steps (denaturation, buffer components, delipidation, etc.)
	Liquid handling methods (automated or manual, technique, equipment, etc.)
<i>Experimental protocols</i>	Array types
	Sample pH and dilution factor
	Quantity of sample loading and position on arrays
	Sample binding, washing and drying procedures
	Matrix addition (type and method)
	Instruments settings
	Number of instruments, locations
<i>Data analysis methods</i>	Environmental factors (temperature, humidity percentage)
	Spectrum processing (baseline subtraction, normalization, alignment, noise reduction, etc.)
	Peak labelling
	Feature selection, statistical analysis
	Classification approaches

fluids are presented in Table 2 as well as formulated recommendations. When reviewing a series of studies [47–49, 51, 54, 57, 58, 60, 61, 67, 68, 73, 81–83, 85] general guidelines can be forwarded. Optimal serum clotting arises after 60 minutes at room temperature. After clot formation, samples can be transported or stored on wet ice for 3 hours before centrifugation. Aliquots must be prepared and stored at -80°C . For plasma collection, anticoagulant EDTA is preferred and its processing should be realized as soon as possible after sampling, ideally within the first hour. Although storage at low temperature promotes peptides and proteins stability, one should not recommend storing plasma samples at 4°C due to the cold activation of platelets. Prior any freezing, plasma can be depleted in platelets by using a filtration step; aliquots are then freeze-dried at -80°C .

According to the “HUPO PPP Specimens Committee” recommendations, plasma appears preferable to serum because it contains less peptides of degradation and consequently presents less variability [57, 81, 86]. In order to avoid the presence of platelet related peptides, the authors also recommend to use platelet-poor plasma obtained by centrifugation followed by a filtration step. However, the choice of serum could be justified when studying diseases related to coagulation abnormalities. Furthermore, it is often more available in sample banks for retrospective studies.

A controversial parameter is the addition of protease inhibitors (PIs) to the samples. Some authors found that the addition of a PI cocktail induces significant differences in protein profiles when compared to crude samples [58, 83]. Whenever directly introduced during phlebotomy, PI allows

TABLE 2: Advantages and limitations of body fluids particularly useful for biomarker discovery.

Body fluids	Advantages	Limitations	Recommendations
Serum	(i) established sample banks often composed of serum aliquots (retrospective studies), (ii) proteins and peptides that “survive” to the clotting procedure exhibit a stability that can be exploited in routine clinical applications.	(i) presence of various products derived from coagulation cascade, (ii) biomarker with poor stability during coagulation process will not be detected in serum, (iii) possible influence of the disease on coagulation process.	(i) use standardized collection protocol, (ii) keep sample during 1 hour at RT to allow clotting process before centrifugation, (iii) preserve on ice after clotting. Aliquoting and freezing (-80°C) cannot be done immediately.
Plasma	(i) more rapidly processed than serum (interesting for emergency diagnosis), (ii) larger final volume of fluid after processing than with serum, (iii) more stable than serum due to the inhibition of coagulation cascade.	(i) interference with chip surface (i.e. heparin tube), (ii) sample dilution in citrate tube, (iii) possible interference of EDTA with protein binding on IMAC surface, (iv) SELDI-TOF spectra less rich in peaks number and intensity than serum.	(i) use standardized collection protocol, (ii) carefully choose the type of anticoagulants (EDTA tubes are preferable), (iii) use platelet-poor plasma, (iv) centrifuge, aliquot and freeze (-80°C) as soon as possible. If not possible, keep at RT to avoid cold platelet activation.
Dry blood	(i) medical staff not needed for collection, (ii) low blood volume necessary, (iii) easy storage and transport.	(i) elution step to recover sample from filter paper.	(i) keep dry specimens at RT for 3–4 hours in horizontal position, (ii) store at -20°C .
Saliva	(i) easy and noninvasive sampling, (ii) medical staff not needed for collection,	(i) low volume collected, (ii) presence of many proteases and unspecific materials such as food residues or microorganisms, (iii) level of certain plasma proteins are not reflected in saliva.	(i) always collect with the same method (stimulated or not) and at the same moment of the day, (ii) centrifuge to remove insoluble material, aliquot and freeze at -80°C .
Urine	(i) easy and noninvasive collection, (ii) medical staff not needed for collection, (iii) obtained in large volume.	(i) fluctuation of protein concentration overtime and according to renal integrity, (ii) presence of salts and proteins in low concentration.	(i) use standardized collection protocol, (ii) concentrate the samples, (iii) centrifuge, aliquot and freeze at -80°C , (iv) normalization with creatinine content.

fluid stabilization for at least 2 hours at room temperature by reducing proteolysis damages. However, PI presents some additional drawbacks such as the presence of highly concentrated components in the cocktail which can compete later on for protein array interactions.

Another important factor to decrease the risk of variation, bias, and errors is the communication between researchers and medical staff. One generally considers that 70% of the errors are due to human intervention (mostly due to communication problems) while only 30% appear instrumental related errors [87]. The mode of specimen collection (veni-puncture or arterial puncture), the site of collection, the position of the patient, or the tourniquet technique can influence the concentration of certain blood constituents [58]. Hemolysis also causes significant changes in blood proteome specimens [67]. It is generally advised to discard those kinds of samples, but when the disease studied involves spontaneous hemolysis, this cannot reasonably be done.

Less commonly used, filter papers were also described to collect blood [68]. This mode of collection has the advantage that only few drops of blood are needed (particularly interesting for neonatal and repeated screening). Moreover, it does not require specific medical support for sampling, which could be promising for multiple collects realized by the patient at home, in the perspective of a treatment follow-up, for instance. Stability and reproducibility of this collection mode remain to be studied.

Saliva and urine have more recently presented an interest in biomarker discovery. Their collection is simple, noninvasive, and cheap and can be easily repeated. However, like blood specimen, such factors have to be taken into consideration to improve reproducibility of sample collection. Saliva protein composition varies with circadian rhythm, diet, age, gender, and physiological status [86]. It is also affected by the method of sample collection (stimulated versus non-stimulated saliva production) [60]. Food ingestion increases the proteolysis activity and then collection before lunch rather than after is recommended [73]. The addition of PI can reduce but not completely eliminate the impact of the proteolysis [60]. It will stabilize, qualitatively and quantitatively, the saliva proteome for up to 48 hours [73]. Regarding storage conditions, it is preferred to store the saliva specimens at -80°C rather than at -20°C where the preservation of the protein content could not be guaranteed for more than 1 month. Interestingly, repeated freeze-thaw cycles (4/5) do not seem to significantly alter saliva protein profile [74].

Urine has the advantage that it can be obtained in large volume. It is mainly an aqueous solution (95% of water) of waste electrolytes and metabolites, organic components (urea, uric acid), and proteins at low concentrations in healthy individuals (150 mg/day). Urine proteome variation depends mainly on plasma composition due to its role as blood content regulator and on the integrity of the glomerular filtration step leading to a large intra and intersubjects variability. Protein and salt concentrations can vary along the day for a same subject (first void compared to midstream urine samples) [80, 88]. Progressive degradation of urine

proteome due to proteolytic activity can be prevented by PI addition only up to 2 hours of storage [54]. As already mentioned for blood and saliva, up to 5 freeze/thaw cycles do not significantly affect urine proteome profile. Storage at -80°C is still requested.

Other fluids such cerebrospinal fluid, nipple aspirates, tears, synovial fluid, bronchoalveolar lavage, follicular, and amniotic fluids have already been explored by SELDI-TOF-MS [15, 20, 33, 34, 69, 75, 89, 90]. These fluids are generally used to study well-localized diseases. Despite the presence in such fluids of some plasma proteins, their implication to study systemic diseases is not recommended and difficult to apply in routine diagnosis due to risk and discomfort related to collection.

3.2. Sample Processing. One of the most challenging aspects in studying body fluids protein profiles remains the detection of the deep proteome [91]. The protein concentration dynamic range detectable by means of MALDI-TOF or SELDI-TOF-MS is about 2 orders of magnitude, whereas the range in blood reaches about 10 orders of magnitude [91, 92]. As protein binding onto chromatographic surface depends on its affinity, its concentration, but also on the surface binding capacity, one can imagine that the competition between different proteins for binding sites is very complex. A highly abundant protein with low affinity for the chip surface and a low abundant protein with high affinity may give similar peak intensities in the final SELDI mass spectrum. Furthermore, protein steric hindrance can also affect the SELDI profiles.

Several fractionation procedures are now available to decrease the sample protein concentration dynamic range [85, 93–102].

A major inconvenience for sample fractionation is the resulting low sample throughput capacity, due to a significant increase of the duration of analysis and to a risk of poor reproducibility affecting data treatment. Use of automatized technologies can improve the reproducibility and decrease the total analysis time. Additionally the same proteins can be presented in different fractions challenging the comparison of their abundance between samples.

Several methods have been proposed for fractionation such as centrifugal ultrafiltration, precipitation by organic solvents, electrophoresis, chromatography (on-column or on-magnetic beads), or subcellular localization. The choice will be made based on the nature of the sample to be analysed and the protein properties (molecular weight, localization, abundance, etc.). All these sample preparation methods have already been discussed by other reviewers [85, 94, 101, 103, 104]. Recently, with the growing interest in studying posttranslational modifications new methodologies set up to isolate rare amino acid-containing peptides (cys, met, trp, his) or PTM peptides (phosphopeptides, glycopeptides) have been developed [25]. One of the most widely used approach for highly abundant proteins removal in serum and plasma is their depletion using antibodies. Despite the depletion of the nine most abundant proteins from serum or plasma samples, overall published results were quite disappointing [105]. This

sensitivity problem is most probably inherent to the too low concentration of the peptidome constituents. Moreover, some of the abundant proteins act as carrier explaining the codepletion of almost 3000 species (peptides and proteins) as observed by several groups [106].

A new fractionation approach has been recently developed by Righetti and Boschetti [107]. It implied a solid-phase combinatorial library of hexapeptides on which millions of copies of a unique ligand are graft on a bead. This technique, enabling the dilution of abundant protein by rapid saturation of its ligand, concentrates components of the deep proteome which could not reach saturation. This method presents the advantage to reduce the dynamic range between the most and less abundant proteins and peptides. It has also been showed that despite compression of the dynamic range, this technology used for differential studies was only applicable for proteins or peptides which do not reach saturation (low and medium abundance proteins) [107]. Many studies conducted on different types of samples report good reproducibility and important gain in the number of low abundant species by comparison with analyses performed on corresponding crude samples [96, 98, 99, 108–111], which make this approach very promising to investigate the deep proteome.

4. SELDI Settings

In order to highlight candidate protein biomarkers, several chromatographic surfaces must be screened. The choice of the protein chip array chemistry and the nature of the matrix depend on whether the application requires general profiling or requires a specific protein assay. Different array types and binding conditions may generate complementary protein profiles for the same sample [7]. The use of relevant quality controls (QCs) is highly recommended and even mandatory in such applications [37–40, 47–63]. QCs should be well-characterized pools of samples processed alongside the experimental samples in order to monitor instrument performances, optimize mass spectrometry settings (laser energy, etc.), compare target protein profiles to those of historical reference samples, and to calculate coefficient of variation for peak intensities as a measure of reproducibility.

It is important to point that the resolution and mass accuracy provided by this kind of instrument are rather low compared to high-resolution mass spectrometers (i.e., Q-TOF, FT-MS, etc.). Using SELDI-TOF-MS, one could not expect to accurately determined m/z values or peak intensities on complex mixtures. Indeed, low resolution causes peaks overlap making abundance and mass assignment difficult. This means that only large differences in peak intensities are to be considered and that peaks of interest have to be identified with more accurate mass spectrometers. Beside those instrumental weaknesses, on the contrary to other mass spectrometers, SELDI-TOF-MS can be used for high throughput analysis.

During SELDI settings, numerous sources of spectra variability have to be taken into account.

Several events, such as matrix crystallization, ion suppression, and in-source decay occurring during mass spectra acquisition strongly influence the peak intensities. These are commented in more details below.

4.1. Matrix Crystallization. Differences in reagents, handling of material, room temperature, and level of humidity may all influence the (co)crystallization step of matrix molecule with sample causing interday fluctuation. The structure and nature of the target surface may also affect peak intensities. These parameters must be highly controlled and standardized for each study protocol. During the crystallization process, a competition phenomenon can occur between proteins for crystal inclusion. Easily embedded proteins will be present at higher concentrations in the matrix and consequently more efficiently desorbed and ionized [47]. To improve sample-to-sample reproducibility of MALDI ion yield and to increase the precision of peptide quantification, some authors use nitrocellulose in order to improve the homogeneity of the matrix/analyte crystallization [55, 112, 113]. This operation might also be helpful for SELDI-TOF-MS measurements.

4.2. Ion Suppression. Depending on sample composition, ion suppression is another factor that significantly contributes to the variability observed in SELDI-TOF-MS spectra [47, 50, 55]. Indeed, during ionization, analytes compete for protons that are transferred from matrix molecules. If a protonated analyte collides with an unprotonated one which has higher gas-phase basicity, it may pass its proton to the collision partner. Therefore, the presence of an analyte may reduce the signal intensity of another. This phenomenon is called “ion suppression effect.” In a complex protein mixture like serum, where highly abundant proteins constitute a large proportion of the total protein content, it is possible that such peaks override signals from low abundant peptides. This phenomenon, obviously difficult to prevent in complex samples, would be more easily controlled on mixtures issued from fractionation.

4.3. In-Source-Decay. Another source of variations is the fragmentation of proteins or peptides during mass spectrometric process. Fragmentation occurring before the first field-free region is called in-source decay (ISD); it is responsible for consecutive series of ions [114].

Ekblad et al. showed that ISD generates quite additional spectral peaks in the spectrum of proteins contained in serum samples when compared with the data collected for pure reference proteins [114]. One obviously creates ISD favourable conditions when optimizing the analytical conditions by maximizing the total peak count, particularly when using a high laser beam which would increase the thermal ions energy and consequently the number of collisions between ions. Hopefully, in-source fragmentation remains quite limited [114]. Dijkstra et al. developed a method which deconvolutes the spectrum by appropriately associating peaks belonging to the same protein [50]. To take benefit

of this procedure, highly efficient sample fractionation is recommended.

4.4. Miscellaneous. Other phenomena susceptible to affect SELDI spectra must be considered. Common mechanisms accounting for the arising of multiple peaks in mass spectra include, for example, the formation of salt adducts and multiply charged ions [50]. Chemical reactions using energy from the laser may take place between sample protein molecules, matrix molecules, or molecules from the washing buffers generating intermolecular complexes known as “ions cluster” [50]. The formation of these complexes increases the number of spectrum peaks causing artefacts (i.e., satellite peak at +206 Da corresponds to a SPA adduct). Moreover, the performance of the SELDI-TOF-MS may change over time due to possible fluctuation in the laser intensity and/or detector sensitivity.

All these difficulties can be addressed only by substantial reduction in sample complexity and the application of a rigorous standardization program of the entire analytical process. This involves optimized acquisition protocols (i.e., avoiding too high laser intensity), a fully operational and calibrated instrument and the use of suitable QC samples, similar in nature and complexity to the studied samples.

5. Data Analysis

5.1. Spectrum Processing. Another important methodological source of artefacts is the data analysis of protein profiles. The data preprocessing (calibration, baseline correction, normalization, peak detection, and peak alignment) represents a key step for SELDI analysis [115–117].

Spectra are generally normalized in order to equalize or minimize differential effect due to external variation [59, 115, 116, 118, 119]. The widely used total ion current (TIC) gives a clear indication of the impacts of technical variables such as laser and detector performances, matrix application, and sample amounts. TIC normalisation relies on the assumption that the technical parameters are mostly responsible for the largest differences observed between samples. But Cairns et al. showed that TIC may also potentially remove some pertinent biological information [115]. They suggest to examine whether normalisation factors vary systematically between study groups and they recommend to specify the applied methodology (local or global normalisation, matrix signal excluded or not). The ideal normalisation procedure would be to resort to some internal spiking method.

5.2. Classification Approaches. One important aspect in SELDI-TOF-MS data analysis is to avoid false discovery of protein peaks, for which the discriminative power results from random variation. A general criticism concerns the use of inadequate algorithms for data analysis and the problem issued from over-adjustment in combination of high-dimensional data with a low number of cases. Those artefacts could be prevented by analysing a sufficient number of samples, by resorting to overfitting-resistant algorithms, by an appropriate validation of the resultant model, and

by using optimal spectra processing techniques (calibration, exclusion of spectral regions affected by high noise, peak alignment, and normalization). Two others remarks can be formulated from literature reports: (1) multiple biomarkers have generally a better predictive value than individual markers, and (2) positive-predictive values of peptide patterns are often insufficient to be recognized as early markers when they concern low-frequency diseases in the population [38, 53].

The most commonly used bioinformatics approaches are decision tree-based ones and support vector machines [120, 121]. Authors generally emphasized on the need for validated model selection using cross validation loop and permutation testing to develop generalized classifier able to correctly predict classification of new samples [122].

6. Biomarkers: From Identification to Clinical Application

Identification of candidate biomarkers, while not strictly necessary for diagnostic purpose, can be regarded as extremely satisfying in helping to data interpretation and better understanding the disease. As often criticized, the SELDI-TOF-MS technology does not provide peptide/protein identification. In order to succeed in the identification by sequencing (Q-TOF, TOF-TOF, ion-trap, etc.) or peptide fingerprinting (MALDI-TOF), enrichment and purification of the biomarker of interest is often needed, which is laborious and time consuming. To solve in part this weakness, new ProteinChip interface coupled to tandem mass spectrometer was recently developed allowing direct sequencing of peptides <6000 Da [124]. In all cases, identifications must be corroborated using antibody-based detection (i.e., Western blot or ELISA) or antibody pull-down with subsequent detection by SELDI-TOF-MS.

It should be noted that the concentration range of widely used biomarkers in plasma samples is remarkably wide and differ from the high milligram until low nanogram per liter range. For example, serum albumin, within a normal concentration range of 35–50 mg/mL, is measured as an indication of severe liver disease [125] or malnutrition [126], whereas IL-6 normally varies in a range of 0–5 pg/mL, is measured as a sensitive indicator of inflammation or infection [127].

Until now, most of the markers identified after an SELDI-TOF-MS study could not yet be considered as very specific of a given disease but they are rather representative of disease's consequences like inflammation or immune response. The most frequently identified proteins so far are haptoglobin, transthyretin, apolipoproteins, serum amyloid, or complement factors present at $\mu\text{g/mL}$ to mg/mL [13, 19, 23–25, 28, 38]. Although individual acute-phase reactions proteins are not satisfactory diagnosis biomarkers, their combined use with other serum biomarkers may enable more sensitive and specific diagnosis (cf., Figure 3). This phenomenon has recently been termed “host response protein amplification cascade” [122]. Acute-phase proteins could also be directly produced by the disease tissue.

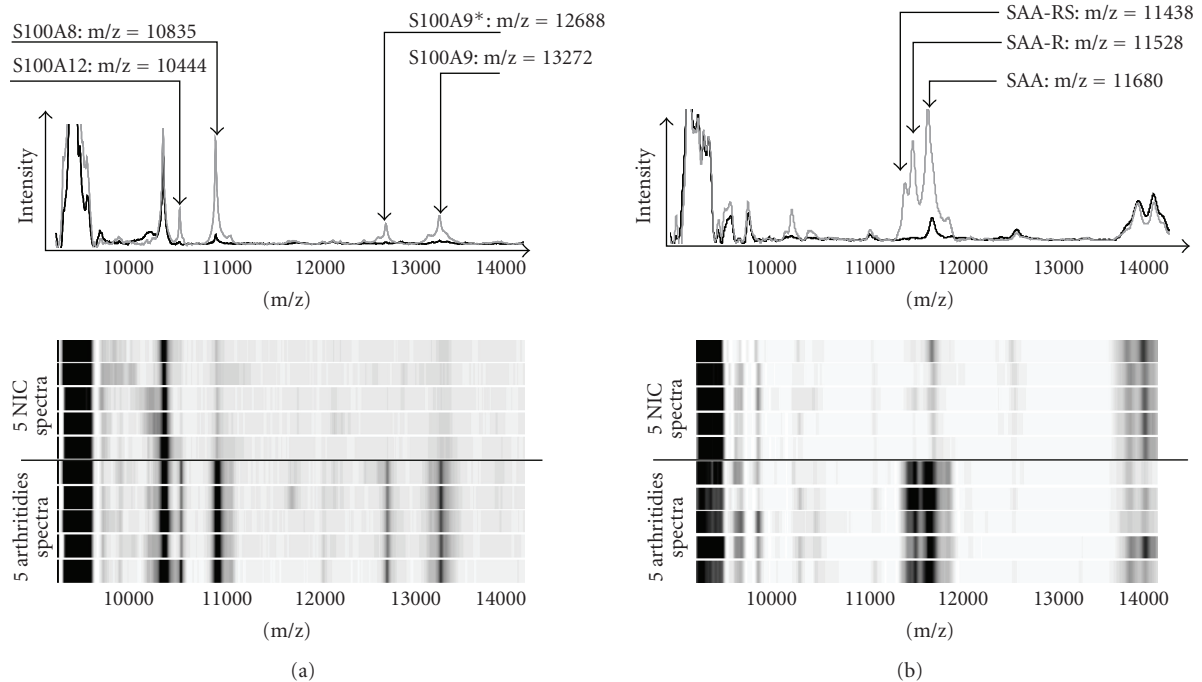


FIGURE 3: Protein mass spectra collected on CM10 and IMAC-Cu²⁺ ProteinChip arrays with serum samples provided by five patients with arthritides (including rheumatoid arthritis, psoriatic arthritis and ankylosing spondylitis) and five noninflammatory controls (NIC) (including osteoarthritis). (a) The inflammatory-related proteins S100A8, S100A12, S100A9, and one of its variant S100A9* are arthritis biomarkers detected on CM10 arrays. (b) On IMAC-Cu²⁺ ProteinChip arrays, SAA and its 2 variants (SAA-R and SAA-RS) are illustrated, reproduced from [19].

The moderate specificity of SELDI-discovered biomarkers could be explained by its low sensibility. To date, SELDI-TOF-MS has not yet identified any protein marker present at ng/mL level. This probably indicates that the lowest detect limit of this technology is around $\mu\text{g/mL}$ as considered by Diamandis [128]. To overcome this limited detection sensitivity, the serum (or plasma) proteins can be fractionated (cf., Section 3.2) before SELDI-TOF-MS analysis. Fractions could then be loaded on different arrays using complementary binding conditions.

Moreover, the decisive advantage of the mass spectrometry technologies is the capacity to detect protein variants, protein fragments, and posttranscriptional modifications (PTMs), which is usually not possible with affinity-based technologies. It is now recognized that those components may be disease-specific and can be considered as potential biomarkers (i.e., modified transthyretin forms in ovarian cancer in Figure 4 and in familial amyloidotic polyneuropathy) [123, 129, 130].

In the last two years, lots of applications using SELDI-TOF-MS were published for diagnostic of cancers [25, 42, 44, 131], especially breast [10, 17], prostate [21, 132, 133], and colorectal cancer [24]. Other recent papers concerning infectious diseases [22], neurodegenerative disorders [35], renal diseases [26, 134], and chronic inflammatory diseases [19, 135] also demonstrated the great potential of the technique.

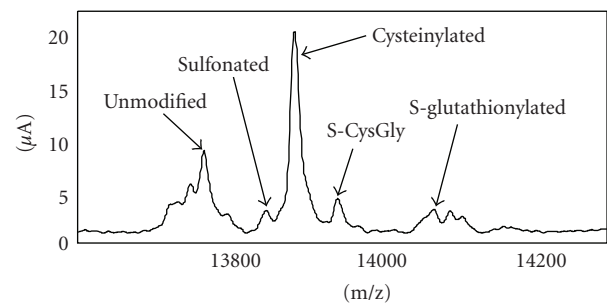


FIGURE 4: Modified transthyretin forms observed in ovarian cancer sample, adapted from [123].

SELDI-TOF-MS technology was also used to predict response to therapy, particularly in cancers. Röcken and Whelan described in detail the use of SELDI-TOF-MS to not only predict responses to cancer therapy but also demonstrate its interest in the follow-up of metastasis disease progression and in the development of drug resistance [44, 136]. Recently platelet factor 4 (PF4) appeared to be a biomarker for Infliximab nonresponse in Crohn's disease and rheumatoid arthritis [29, 137].

For most of these studies, a validation phase should assess the validity of the described potential biomarkers against a larger and more heterogeneous population of patients. The

robustness of the candidate markers has to be tested against a level of biological variability that more accurately reflects the variability in the target population.

Unfortunately, several groups failed to validate the biomarker discovered in their pilot study, such as McLerran et al. [39, 40], and others [36, 66]. McLerran et al. described preanalytical bias. They concluded that their first study samples most likely had biases in the sample selection. Another validation performed by Engwegen et al. using distinct patient populations confirmed that SAA peak clusters are associated to renal cell carcinoma. However, some other markers could not be validated [36]. Such examples demonstrate the importance to strictly control parameters such as storage, clotting, time of analysis, instrument performances, sample selection, and statistical classification method.

The urgent need for SOPs in clinical proteomics research is therefore absolutely mandatory reflecting a growing trend in the field [19, 53, 62, 63]. Interaction between researchers, clinicians, and statisticians is also a key element for the success.

Altogether, these applications of SELDI-TOF-MS technology illustrate its capability for discrimination and follow-up of a multitude of diseases using different body fluids as well as certain therapeutic response prediction. It is worth mentioning that FDA approved recently the first diagnostic tool (named OVA1) issued from SELDI proteomic researches. It is made of the combination of 5 markers for ovarian cancer diagnostic.

7. Concluding Remarks

Taking into account herein and previously described recommendations, SELDI-TOF-MS offers very exciting opportunities to discover not only diagnostic but also prognostic and mechanistic markers for a number of major diseases.

To face the general criticism, standardized procedures and recommendations to minimize bias are now followed by most of the users. However, some challenges still remain, as for all other proteomic approaches, due in part to the complexity and the wide dynamic range of the samples. Sample fractionation and/or enrichment procedure, such as peptide ligand affinity beads, will certainly be the solution to visualise the deep proteome. In addition, improvements in mass spectrometry instrumental performances could be expected (higher resolution, reducing adduct formation, and ion suppression), contributing further to more reliable and faster biomarkers discovery.

Abbreviations

2-DE:	Two-dimensional electrophoresis
CSF:	Cerebrospinal fluid
EDTA:	Ethylenediaminetetraacetic acid
ELISA:	Enzyme-Linked Immunosorbent Assay

HUPO PPP	Plasma Proteome Project
Specimens Committee:	
IMAC:	Immobilized Metal Affinity Capture
ISD:	In-Source Decay
LC-MS:	Liquid Chromatography—Mass Spectrometry
MALDI-TOF:	Matrix-Assisted Laser Desorption/Ionisation—Time-Of-Flight
PI:	Protease inhibitor
PTM:	Post-translational modifications
PSA:	Prostate specific antigen
QC:	Quality control
SELDI-TOF-MS:	Surface-Enhanced Laser Desorption/Ionisation—Time-Of-Flight—Mass Spectrometry
SOP:	Standard Operating Procedures
SPA:	Sinapic acid
SVM:	Support Vector Machine
TIC:	Total Ion Current.

Acknowledgment

The authors thank Jean De Graeve for his advices. M. Fillet is a Research Associate; M.P. Merville and E. Louis are Senior Research Associates at the FNRS (National Fund for Scientific Research, Belgium).

References

- [1] L. A. Liotta, M. Ferrari, and E. Petricoin, "Clinical proteomics: written in blood," *Nature*, vol. 425, no. 6961, p. 905, 2003.
- [2] A. D. Westont and L. Hood, "Systems biology, proteomics, and the future of health care: toward predictive, preventative, and personalized medicine," *Journal of Proteome Research*, vol. 3, no. 2, pp. 179–196, 2004.
- [3] A. Gorg, W. Weiss, and M. J. Dunn, "Current two-dimensional electrophoresis technology for proteomics," *Proteomics*, vol. 4, no. 12, pp. 3665–3685, 2004.
- [4] G. Mitulovic, C. Stingl, M. Smoluch, et al., "Automated, on-line two-dimensional nano liquid chromatography tandem mass spectrometry for rapid analysis of complex protein digests," *Proteomics*, vol. 4, no. 9, pp. 2545–2557, 2004.
- [5] R. S. Tirumalai, K. C. Chan, D. A. Prieto, H. J. Issaq, T. P. Conrads, and T. D. Veenstra, "Characterization of the low molecular weight human serum proteome," *Molecular & Cellular Proteomics*, vol. 2, no. 10, pp. 1096–1103, 2003.
- [6] G. L. Wright Jr., "SELDI proteinchip MS: a platform for biomarker discovery and cancer diagnosis," *Expert Review of Molecular Diagnostics*, vol. 2, no. 6, pp. 549–563, 2002.
- [7] T. Hutchens and T. Yip, "New desorption strategies for the mass spectrometric analysis of macromolecules," *Rapid Commun Mass Spectrom*, vol. 7, pp. 576–580, 1993.
- [8] G. L. Wright Jr., L. H. Cazares, S.-M. Leung, et al., "ProteinChip® surface enhanced laser desorption/ionization (SELDI) mass spectrometry: a novel protein biochip technology for detection of prostate

- cancer biomarkers in complex protein mixtures,” *Prostate Cancer and Prostatic Diseases*, vol. 2, no. 5-6, pp. 264–276, 1999.
- [9] N. Tang, P. Tornatore, and S. R. Weinberger, “Current developments in SELDI affinity technology,” *Mass Spectrometry Reviews*, vol. 23, no. 1, pp. 34–44, 2004.
 - [10] M. Abramovitz and B. Leyland-Jones, “A systems approach to clinical oncology: focus on breast cancer,” *Proteome Science*, vol. 4, p. 5, 2006.
 - [11] F. Bertucci, D. Birnbaum, and A. Goncalves, “Proteomics of breast cancer: principles and potential clinical applications,” *Molecular and Cellular Proteomics*, vol. 5, no. 10, pp. 1772–1786, 2006.
 - [12] F. Bertucci and A. Goncalves, “Clinical proteomics and breast cancer: strategies for diagnostic and therapeutic biomarker discovery,” *Future Oncology*, vol. 4, no. 2, pp. 271–287, 2008.
 - [13] J. A. P. Bons, M. P. van Diejen-Visser, and W. K. W. H. Wodzig, “Clinical proteomics in chronic inflammatory diseases: a review,” *Proteomics Clinical Applications*, vol. 1, no. 9, pp. 1123–1133, 2007.
 - [14] C. S. Buhimschi, V. Bhandari, B. D. Hamar, et al., “Proteomic profiling of the amniotic fluid to detect inflammation, infection, and neonatal sepsis,” *PLoS Medicine*, vol. 4, no. 1, article e18, 2007.
 - [15] I. A. Buhimschi, E. Zambrano, C. M. Pettker, et al., “Using proteomic analysis of the human amniotic fluid to identify histologic chorioamnionitis,” *Obstetrics and Gynecology*, vol. 111, no. 2, part 1, pp. 403–412, 2008.
 - [16] I. A. Buhimschi, G. Zhao, V. A. Rosenberg, S. Abdel-Razek, S. Thung, and C. S. Buhimschi, “Multidimensional proteomics analysis of amniotic fluid to provide insight into the mechanisms of idiopathic preterm birth,” *PLoS ONE*, vol. 3, no. 4, article e2049, 2008.
 - [17] C. H. Clarke, J. A. Buckley, and E. T. Fung, “SELDI-TOF-MS proteomics of breast cancer,” *Clinical Chemistry and Laboratory Medicine*, vol. 43, no. 12, pp. 1314–1320, 2005.
 - [18] D. de Seny, M. Fillet, M.-A. Meuwis, et al., “Discovery of new rheumatoid arthritis biomarkers using the surface-enhanced laser desorption/ionization time-of-flight mass spectrometry proteinchip approach,” *Arthritis and Rheumatism*, vol. 52, no. 12, pp. 3801–3812, 2005.
 - [19] D. de Seny, M. Fillet, C. Ribbens, et al., “Monomeric calgranulins measured by SELDI-TOF mass spectrometry and calprotectin measured by ELISA as biomarkers in arthritis,” *Clinical Chemistry*, vol. 54, no. 6, pp. 1066–1075, 2008.
 - [20] J. He, J. Gornbein, D. Shen, et al., “Detection of breast cancer biomarkers in nipple aspirate fluid by SELDI-TOF and their identification by combined liquid chromatography-tandem mass spectrometry,” *International Journal of Oncology*, vol. 30, no. 1, pp. 145–154, 2007.
 - [21] M. Hellstrom, H. Lexander, B. Franzen, and L. Egevad, “Proteomics in prostate cancer research,” *Analytical and Quantitative Cytology and Histology*, vol. 29, no. 1, pp. 32–40, 2007.
 - [22] A. Hodgetts, M. Levin, J. S. Kroll, and P. R. Langford, “Biomarker discovery in infectious diseases using SELDI,” *Future Microbiology*, vol. 2, no. 1, pp. 35–49, 2007.
 - [23] J. T.-J. Huang, L. Wang, S. Prabakaran, et al., “Independent protein-profiling studies show a decrease in apolipoprotein A1 levels in schizophrenia CSF, brain and peripheral tissues,” *Molecular Psychiatry*, vol. 13, no. 12, pp. 1118–1128, 2008.
 - [24] S. Hundt, U. Haug, and H. Brenner, “Blood markers for early detection of colorectal cancer: a systematic review,” *Cancer Epidemiology Biomarkers and Prevention*, vol. 16, no. 10, pp. 1935–1953, 2007.
 - [25] K. K. Jain, “Recent advances in clinical oncoproteomics,” *Journal of Buon*, vol. 12, supplement 1, pp. S31–S38, 2007.
 - [26] Y. Mao, J. Yu, J. Chen, et al., “Diagnosis of renal allograft subclinical rejection by urine protein fingerprint analysis,” *Transplant Immunology*, vol. 18, no. 3, pp. 255–259, 2008.
 - [27] R. Martinez-Pinna, J. L. Martin-Ventura, S. Mas, L. M. Blanco-Colio, J. Tunon, and J. Egido, “Proteomics in atherosclerosis,” *Current Atherosclerosis Reports*, vol. 10, no. 3, pp. 209–215, 2008.
 - [28] M.-A. Meuwis, M. Fillet, P. Geurts, et al., “Biomarker discovery for inflammatory bowel disease, using proteomic serum profiling,” *Biochemical Pharmacology*, vol. 73, no. 9, pp. 1422–1433, 2007.
 - [29] M.-A. Meuwis, M. Fillet, L. Lutteri, et al., “Proteomics for prediction and characterization of response to infliximab in Crohn’s disease: a pilot study,” *Clinical Biochemistry*, vol. 41, no. 12, pp. 960–967, 2008.
 - [30] S. J. Pitteri and S. M. Hanash, “Proteomic approaches for cancer biomarker discovery in plasma,” *Expert Review of Proteomics*, vol. 4, no. 5, pp. 589–590, 2007.
 - [31] E. R. Sauter, S. Shan, J. E. Hewett, P. Speckman, and G. C. Du Bois, “Proteomic analysis of nipple aspirate fluid using SELDI-TOF-MS,” *International Journal of Cancer*, vol. 114, no. 5, pp. 791–796, 2005.
 - [32] Y. Shen, J. Kim, E. F. Strittmatter, et al., “Characterization of the human blood plasma proteome,” *Proteomics*, vol. 5, no. 15, pp. 4034–4045, 2005.
 - [33] A. H. Simonsen, J. McGuire, V. N. Podust, et al., “Identification of a novel panel of cerebrospinal fluid biomarkers for Alzheimer’s disease,” *Neurobiology of Aging*, vol. 29, no. 7, pp. 961–968, 2008.
 - [34] N. Tomosugi, K. Kitagawa, N. Takahashi, S. Sugai, and I. Ishikawa, “Diagnostic potential of tear proteomic patterns in Sjogren’s syndrome,” *Journal of Proteome Research*, vol. 4, no. 3, pp. 820–825, 2005.
 - [35] H. Zetterberg, U. Ruettschi, E. Portelius, et al., “Clinical proteomics in neurodegenerative disorders,” *Acta Neurologica Scandinavica*, vol. 118, no. 1, pp. 1–11, 2008.
 - [36] J. Y. M. N. Engwegen, N. Mehra, J. B. A. G. Haanen, et al., “Validation of SELDI-TOF MS serum protein profiles for renal cell carcinoma in new populations,” *Laboratory Investigation*, vol. 87, no. 2, pp. 161–172, 2007.
 - [37] D. M. Good, V. Thongboonkerd, J. Novak, et al., “Body fluid proteomics for biomarker discovery: lessons from the past hold the key to success in the future,” *Journal of Proteome Research*, vol. 6, no. 12, pp. 4549–4555, 2007.
 - [38] M. Kiehnopf, R. Siegmund, and T. Deufel, “Use of SELDI-TOF mass spectrometry for identification of new biomarkers: potential and limitations,” *Clinical Chemistry and Laboratory Medicine*, vol. 45, no. 11, pp. 1435–1449, 2007.
 - [39] D. McLerran, W. E. Grizzle, Z. Feng, et al., “Analytical validation of serum proteomic profiling for diagnosis of prostate cancer: sources of sample bias,” *Clinical Chemistry*, vol. 54, no. 1, pp. 44–52, 2008.
 - [40] D. McLerran, W. E. Grizzle, Z. Feng, et al., “SELDI-TOF MS whole serum proteomic profiling with IMAC surface does not reliably detect prostate cancer,” *Clinical Chemistry*, vol. 54, no. 1, pp. 53–60, 2008.
 - [41] A. Villar-Garea, M. Griese, and A. Imhof, “Biomarker discovery from body fluids using mass spectrometry,” *Journal of Chromatography B*, vol. 849, no. 1-2, pp. 105–114, 2007.

- [42] P. Maurya, P. Meleady, P. Dowling, and M. Clynes, "Proteomic approaches for serum biomarker discovery in cancer," *Anticancer Research*, vol. 27, no. 3A, pp. 1247–1255, 2007.
- [43] T. L. Nickolas, J. Barasch, and P. Devarajan, "Biomarkers in acute and chronic kidney disease," *Current Opinion in Nephrology and Hypertension*, vol. 17, no. 2, pp. 127–132, 2008.
- [44] L. C. Whelan, K. A. R. Power, D. T. McDowell, J. Kennedy, and W. M. Gallagher, "Applications of SELDI-MS technology in oncology," *Journal of Cellular and Molecular Medicine*, vol. 12, no. 5, pp. 1535–1547, 2008.
- [45] P. Findeisen and M. Neumaier, "Mass spectrometry based proteomics profiling as diagnostic tool in oncology: current status and future perspective," *Clinical Chemistry and Laboratory Medicine*, vol. 47, no. 6, pp. 666–684, 2009.
- [46] R. Apweiler, C. Aslanidis, T. Deufel, et al., "Approaching clinical proteomics: current state and future fields of application in fluid proteomics," *Clinical Chemistry and Laboratory Medicine*, vol. 47, no. 6, pp. 724–744, 2009.
- [47] J. Albrechtsen, R. Bogebo, J. Olsen, H. Raskov, and S. Gammeltoft, "Preanalytical and analytical variation of surface-enhanced laser desorption/ionization time-of-flight mass spectrometry of human serum," *Clinical Chemistry and Laboratory Medicine*, vol. 44, no. 10, pp. 1243–1252, 2006.
- [48] R. E. Banks, A. J. Stanley, D. A. Cairns, et al., "Influences of blood sample processing on low-molecular-weight proteome identified by surface-enhanced laser desorption/ionization mass spectrometry," *Clinical Chemistry*, vol. 51, no. 9, pp. 1637–1649, 2005.
- [49] S. Barelli, D. Cretzaz, L. Thadikkaran, O. Rubin, and J.-D. Tissot, "Plasma/serum proteomics: pre-analytical issues," *Expert Review of Proteomics*, vol. 4, no. 3, pp. 363–370, 2007.
- [50] M. Dijkstra, R. J. Vonk, and R. C. Jansen, "SELDI-TOF mass spectra: a view on sources of variation," *Journal of Chromatography B*, vol. 847, no. 1, pp. 12–23, 2007.
- [51] G. L. Hortin, "Can mass spectrometric protein profiling meet desired standards of clinical laboratory practice?" *Clinical Chemistry*, vol. 51, no. 1, pp. 3–5, 2005.
- [52] J. N. McGuire, J. Overgaard, and F. Pociot, "Mass spectrometry is only one piece of the puzzle in clinical proteomics," *Briefings in Functional Genomics and Proteomics*, vol. 7, no. 1, pp. 74–83, 2008.
- [53] H. Mischak, R. Apweiler, R. E. Banks, et al., "Clinical proteomics: a need to define the field and to begin to set adequate standards," *Proteomics Clinical Applications*, vol. 1, no. 2, pp. 148–156, 2007.
- [54] M. Papale, M. C. Pedicillo, B. J. Thatcher, et al., "Urine profiling by SELDI-TOF/MS: monitoring of the critical steps in sample collection, handling and analysis," *Journal of Chromatography B*, vol. 856, no. 1–2, pp. 205–213, 2007.
- [55] T. C. W. Poon, "Opportunities and limitations of SELDI-TOF-MS in biomedical research: practical advices," *Expert Review of Proteomics*, vol. 4, no. 1, pp. 51–65, 2007.
- [56] A. J. Rai, C. A. Gelfand, B. C. Haywood, et al., "HUPO plasma proteome project specimen collection and handling: towards the standardization of parameters for plasma proteome samples," *Proteomics*, vol. 5, no. 13, pp. 3262–3277, 2005.
- [57] A. J. Rai, P. M. Stemmer, Z. Zhang, et al., "Analysis of human proteome organization plasma proteome project (HUPO PPP) reference specimens using surface enhanced laser desorption/ionization-time of flight (SELDI-TOF) mass spectrometry: multi-institution correlation of spectra and identification of biomarkers," *Proteomics*, vol. 5, no. 13, pp. 3467–3474, 2005.
- [58] A. J. Rai and F. Vitzthum, "Effects of preanalytical variables on peptide and protein measurements in human serum and plasma: implications for clinical proteomics," *Expert Review of Proteomics*, vol. 3, no. 4, pp. 409–426, 2006.
- [59] D. Rollin, T. Whistler, and S. D. Vernon, "Laboratory methods to improve SELDI peak detection and quantitation," *Proteome Science*, vol. 5, p. 9, 2007.
- [60] R. Schipper, A. Loof, J. de Groot, L. Harthoorn, E. Dransfield, and W. van Heerde, "SELDI-TOF-MS of saliva: methodology and pre-treatment effects," *Journal of Chromatography B*, vol. 847, no. 1, pp. 45–53, 2007.
- [61] J. F. Timms, E. Arslan-Low, A. Gentry-Maharaj, et al., "Preanalytic influence of sample handling on SELDI-TOF serum protein profiles," *Clinical Chemistry*, vol. 53, no. 4, pp. 645–656, 2007.
- [62] C. N. White, Z. Zhang, and D. W. Chan, "Quality control for SELDI analysis," *Clinical Chemistry and Laboratory Medicine*, vol. 43, no. 2, pp. 125–126, 2005.
- [63] O. J. Semmes, Z. Feng, B.-L. Adam, et al., "Evaluation of serum protein profiling by surface-enhanced laser desorption/ionization time-of-flight mass spectrometry for the detection of prostate cancer: I. Assessment of platform reproducibility," *Clinical Chemistry*, vol. 51, no. 1, pp. 102–112, 2005.
- [64] K. A. Baggerly, J. S. Morris, and K. R. Coombes, "Reproducibility of SELDI-TOF protein patterns in serum: comparing datasets from different experiments," *Bioinformatics*, vol. 20, no. 5, pp. 777–785, 2004.
- [65] J. Hu, K. R. Coombes, J. S. Morris, and K. A. Baggerly, "The importance of experimental design in proteomic mass spectrometry experiments: some cautionary tales," *Briefings in Functional Genomics and Proteomics*, vol. 3, no. 4, pp. 322–331, 2005.
- [66] J. Hu, K. R. Coombes, J. S. Morris, and K. A. Baggerly, "The importance of experimental design in proteomic mass spectrometry experiments: some cautionary tales," *Briefings in Functional Genomics and Proteomics*, vol. 3, no. 4, pp. 322–331, 2005.
- [67] S.-Y. Hsieh, R.-K. Chen, Y.-H. Pan, and H.-L. Lee, "Systematical evaluation of the effects of sample collection procedures on low-molecular-weight serum/plasma proteome profiling," *Proteomics*, vol. 6, no. 10, pp. 3189–3198, 2006.
- [68] C. E. L. Dammann, M. Meyer, O. Dammann, and N. von Neuhoff, "Protein detection in dried blood by surface-enhanced laser desorption/ionization-time of flight mass spectrometry (SELDI-TOF MS)," *Biology of the Neonate*, vol. 89, no. 2, pp. 126–132, 2006.
- [69] F. H. Grus, V. N. Podust, K. Bruns, et al., "SELDI-TOF-MS ProteinChip array profiling of tears from patients with dry eye," *Investigative Ophthalmology and Visual Science*, vol. 46, no. 3, pp. 863–876, 2005.
- [70] S. Hu, J. A. Loo, and D. T. Wong, "Human body fluid proteome analysis," *Proteomics*, vol. 6, no. 23, pp. 6326–6353, 2006.
- [71] J. L. Noble, R. S. Dua, G. R. Coulton, C. M. Isacke, and G. P. H. Gui, "A comparative proteomic analysis of nipple aspiration fluid from healthy women and women with breast cancer," *European Journal of Cancer*, vol. 43, no. 16, pp. 2315–2320, 2007.
- [72] E. O'Riordan, T. N. Orlova, V. N. Podust, et al., "Characterization of urinary peptide biomarkers of acute rejection in renal allografts," *American Journal of Transplantation*, vol. 7, no. 4, pp. 930–940, 2007.

- [73] M. Papale, M. C. Pedicillo, S. Di Paolo, et al., "Saliva analysis by surface-enhanced laser desorption/ionization time-of-flight mass spectrometry (SELDI-TOF/MS): from sample collection to data analysis," *Clinical Chemistry and Laboratory Medicine*, vol. 46, no. 1, pp. 89–99, 2008.
- [74] R. Schipper, A. Loof, J. de Groot, L. Harthoorn, W. van Heerde, and E. Dransfield, "Salivary protein/peptide profiling with SELDI-TOF-MS," *Annals of the New York Academy of Sciences*, vol. 1098, pp. 498–503, 2007.
- [75] F. J. Schweigert, B. Gericke, W. Wolfram, U. Kaisers, and J. W. Dudenhausen, "Peptide and protein profiles in serum and follicular fluid of women undergoing IVF," *Human Reproduction*, vol. 21, no. 11, pp. 2960–2968, 2006.
- [76] K. S. Shores and D. R. Knapp, "Assessment approach for evaluating high abundance protein depletion methods for cerebrospinal fluid (CSF) proteomic analysis," *Journal of Proteome Research*, vol. 6, no. 9, pp. 3739–3751, 2007.
- [77] M. Suzuki, G. F. Ross, K. Wiers, et al., "Identification of a urinary proteomic signature for lupus nephritis in children," *Pediatric Nephrology*, vol. 22, no. 12, pp. 2047–2057, 2007.
- [78] A. Goncalves, E. Charafe-Jauffret, F. Bertucci, et al., "Protein profiling of human breast tumor cells identifies novel biomarkers associated with molecular subtypes," *Molecular and Cellular Proteomics*, vol. 7, no. 8, pp. 1420–1433, 2008.
- [79] C. Jansen, K. M. Hebeda, M. Linkels, et al., "Protein profiling of B-cell lymphomas using tissue biopsies: a potential tool for small samples in pathology," *Cellular Oncology*, vol. 30, no. 1, pp. 27–38, 2008.
- [80] S. Schaub, J. Wilkins, T. Weiler, K. Sangster, D. Rush, and P. Nickerson, "Urine protein profiling with surface-enhanced laser-desorption/ionization time-of-flight mass spectrometry," *Kidney International*, vol. 65, no. 1, pp. 323–332, 2004.
- [81] H. Tammen, I. Schulte, R. Hess, et al., "Peptidomic analysis of human blood specimens: comparison between plasma specimens and serum by differential peptide display," *Proteomics*, vol. 5, no. 13, pp. 3414–3422, 2005.
- [82] A. Z. Traum, M. P. Wells, M. Aivado, T. A. Libermann, M. F. Ramoni, and A. D. Schachter, "SELDI-TOF MS of quadruplicate urine and serum samples to evaluate changes related to storage conditions," *Proteomics*, vol. 6, no. 5, pp. 1676–1680, 2006.
- [83] J. Yi, C. Kim, and C. A. Gelfand, "Inhibition of intrinsic proteolytic activities moderates preanalytical variability and instability of human plasma," *Journal of Proteome Research*, vol. 6, no. 5, pp. 1768–1781, 2007.
- [84] A. E. Pelzer, I. Feuerstein, C. Fuchsberger, et al., "Influence of blood sampling on protein profiling and pattern analysis using matrix-assisted laser desorption/ionisation mass spectrometry," *BJU International*, vol. 99, no. 3, pp. 658–662, 2007.
- [85] J. L. Luque-Garcia and T. A. Neubert, "Sample preparation for serum/plasma profiling and biomarker identification by mass spectrometry," *Journal of Chromatography A*, vol. 1153, no. 1–2, pp. 259–276, 2007.
- [86] M. Battino, M. S. Ferreiro, I. Gallardo, H. N. Newman, and P. Bullon, "The antioxidant capacity of saliva," *Journal of Clinical Periodontology*, vol. 29, no. 3, pp. 189–194, 2002.
- [87] H. Voorbij, "Pouten en risico's in een klinisch-chemisch laboratorium," *Nederlands Tijdschrift voor Klinische Chemie*, vol. 19, pp. 36–41, 1994.
- [88] A. Gagnon, Q. Shi, and B. Ye, "Surface-enhanced laser desorption/ionization mass spectrometry for protein and peptide profiling of body fluids," *Methods in Molecular Biology*, vol. 441, pp. 41–56, 2008.
- [89] G. MacGregor, R. D. Gray, T. N. Hilliard, et al., "Biomarkers for cystic fibrosis lung disease: application of SELDI-TOF mass spectrometry to BAL fluid," *Journal of Cystic Fibrosis*, vol. 7, no. 5, pp. 352–358, 2008.
- [90] J. T.-J. Huang, L. Wang, S. Prabakaran, et al., "Independent protein-profiling studies show a decrease in apolipoprotein A1 levels in schizophrenia CSF, brain and peripheral tissues," *Molecular Psychiatry*, vol. 13, no. 12, pp. 1118–1128, 2008.
- [91] N. L. Anderson and N. G. Anderson, "The human plasma proteome: history, character, and diagnostic prospects," *Molecular & Cellular Proteomics*, vol. 1, no. 11, pp. 845–867, 2002.
- [92] M. A. Gillette, D. R. Mani, and S. A. Carr, "Place of pattern in proteomic biomarker discovery," *Journal of Proteome Research*, vol. 4, no. 4, pp. 1143–1154, 2005.
- [93] M. K. D. R. Dayarathna, W. S. Hancock, and M. Hincapie, "A two step fractionation approach for plasma proteomics using immunodepletion of abundant proteins and multi-lectin affinity chromatography: application to the analysis of obesity, diabetes, and hypertension diseases," *Journal of Separation Science*, vol. 31, no. 6–7, pp. 1156–1166, 2008.
- [94] X. Jiang, M. Ye, and H. Zou, "Technologies and methods for sample pretreatment in efficient proteome and peptidome analysis," *Proteomics*, vol. 8, no. 4, pp. 686–705, 2008.
- [95] P. Matt, Z. Fu, Q. Fu, and J. E. Van Eyk, "Biomarker discovery: proteome fractionation and separation in biological samples," *Physiological Genomics*, vol. 33, no. 1, pp. 12–17, 2008.
- [96] M. Pernemalm, L. M. Orre, J. Lengqvist, et al., "Evaluation of three principally different intact protein prefractionation methods for plasma biomarker discovery," *Journal of Proteome Research*, vol. 7, no. 7, pp. 2712–2722, 2008.
- [97] P. G. Righetti, E. Boschetti, L. Lomas, and A. Citterio, "Protein equalizer technology: the quest for a "democratic proteome,"" *Proteomics*, vol. 6, no. 14, pp. 3980–3992, 2006.
- [98] K. S. Shores, D. G. Udugamasooriya, T. Kodadek, and D. R. Knapp, "Use of peptide analogue diversity library beads for increased depth of proteomic analysis: application to cerebrospinal fluid," *Journal of Proteome Research*, vol. 7, no. 5, pp. 1922–1931, 2008.
- [99] C. Sihlbom, I. Kanmert, H. V. Bahr, and P. Davidsson, "Evaluation of the combination of bead technology with SELDI-TOF-MS and 2-D DIGE for detection of plasma proteins," *Journal of Proteome Research*, vol. 7, no. 9, pp. 4191–4198, 2008.
- [100] S. W. Tam, J. Pirro, and D. Hinerfeld, "Depletion and fractionation technologies in plasma proteomic analysis," *Expert Review of Proteomics*, vol. 1, no. 4, pp. 411–420, 2004.
- [101] J. R. Whiteaker, H. Zhang, J. K. Eng, et al., "Head-to-head comparison of serum fractionation techniques," *Journal of Proteome Research*, vol. 6, no. 2, pp. 828–836, 2007.
- [102] F. E. Ahmed, "Sample preparation and fractionation for proteome analysis and cancer biomarker discovery by mass spectrometry," *Journal of Separation Science*, vol. 32, no. 5–6, pp. 771–798, 2009.
- [103] N. Zolotarjova, P. Mrozinski, H. Chen, and J. Martosella, "Combination of affinity depletion of abundant proteins and reversed-phase fractionation in proteomic analysis of human plasma/serum," *Journal of Chromatography A*, vol. 1189, no. 1–2, pp. 332–338, 2008.
- [104] M. Pernemalm, R. Lewensohn, and J. Lehtio, "Affinity pre-fractionation for MS-based plasma proteomics," *Proteomics*, vol. 9, no. 6, pp. 1420–1427, 2009.

- [105] P. G. Righetti and E. Boschetti, "Sherlock Holmes and the proteome—a detective story," *FEBS Journal*, vol. 274, no. 4, pp. 897–905, 2007.
- [106] L. A. Liotta and E. F. Petricoin, "Serum peptidome for cancer detection: spinning biologic trash into diagnostic gold," *The Journal of Clinical Investigation*, vol. 116, no. 1, pp. 26–30, 2006.
- [107] P. G. Righetti and E. Boschetti, "The ProteoMiner and the FortyNiners: searching for gold nuggets in the proteomic arena," *Mass Spectrometry Reviews*, vol. 27, no. 6, pp. 596–608, 2008.
- [108] A. Castagna, D. Cecconi, L. Sennels, et al., "Exploring the hidden human urinary proteome via ligand library beads," *Journal of Proteome Research*, vol. 4, no. 6, pp. 1917–1930, 2005.
- [109] L. Guerrier, S. Claverol, F. Fortis, et al., "Exploring the platelet proteome via combinatorial, hexapeptide ligand libraries," *Journal of Proteome Research*, vol. 6, no. 11, pp. 4290–4303, 2007.
- [110] L. Sennels, M. Salek, L. Lomas, E. Boschetti, P. G. Righetti, and J. Rappsilber, "Proteomic analysis of human blood serum using peptide library beads," *Journal of Proteome Research*, vol. 6, no. 10, pp. 4055–4062, 2007.
- [111] V. Thulasiraman, S. Lin, L. Gheorghiu, et al., "Reduction of the concentration difference of proteins in biological liquids using a library of combinatorial ligands," *Electrophoresis*, vol. 26, no. 18, pp. 3561–3571, 2005.
- [112] J. Albrechtsen, "Reproducibility in protein profiling by MALDI-TOF mass spectrometry," *Clinical Chemistry*, vol. 53, no. 5, pp. 852–858, 2007.
- [113] L. M. Preston, K. K. Murray, and D. H. Russell, "Reproducibility and quantitation of matrix-assisted laser desorption/ionization mass spectrometry: effects of nitrocellulose on peptide ion yields," *Biological Mass Spectrometry*, vol. 22, no. 9, pp. 544–550, 1993.
- [114] L. Ekblad, B. Baldetorp, M. Ferno, H. Olsson, and C. Bratt, "In-source decay causes artifacts in SELDI-TOF MS spectra," *Journal of Proteome Research*, vol. 6, no. 4, pp. 1609–1614, 2007.
- [115] D. A. Cairns, D. Thompson, D. N. Perkins, A. J. Stanley, P. J. Selby, and R. E. Banks, "Proteomic profiling using mass spectrometry—does normalising by total ion current potentially mask some biological differences?" *Proteomics*, vol. 8, no. 1, pp. 21–27, 2008.
- [116] W. Meuleman, J. Y. M. N. Engwegen, M.-C. W. Gast, J. H. Beijnen, M. J. T. Reinders, and L. F. A. Wessels, "Comparison of normalisation methods for surface-enhanced laser desorption and ionisation (SELDI) time-of-flight (TOF) mass spectrometry data," *BMC Bioinformatics*, vol. 9, article 88, 2008.
- [117] W. Wegdam, P. D. Moerland, M. R. Buist, et al., "Classification-based comparison of pre-processing methods for interpretation of mass spectrometry generated clinical datasets," *Proteome Science*, vol. 7, p. 19, 2009.
- [118] N. Jeffries, "Algorithms for alignment of mass spectrometry proteomic data," *Bioinformatics*, vol. 21, no. 14, pp. 3066–3073, 2005.
- [119] C. S. Tan, A. Ploner, A. Quandt, J. Lehtio, and Y. Pawitan, "Finding regions of significance in SELDI measurements for identifying protein biomarkers," *Bioinformatics*, vol. 22, no. 12, pp. 1515–1523, 2006.
- [120] F. M. Smith, W. M. Gallagher, E. Fox, et al., "Combination of SELDI-TOF-MS and data mining provides early-stage response prediction for rectal tumors undergoing multimodal neoadjuvant therapy," *Annals of Surgery*, vol. 245, no. 2, pp. 259–266, 2007.
- [121] P. Geurts, M. Fillet, D. de Seny, et al., "Proteomic mass spectra classification using decision tree based ensemble methods," *Bioinformatics*, vol. 21, no. 14, pp. 3138–3145, 2005.
- [122] S. Smit, H. C. J. Hoefsloot, and A. K. Smilde, "Statistical data processing in clinical proteomics," *Journal of Chromatography B*, vol. 866, no. 1–2, pp. 77–88, 2008.
- [123] E. T. Fung, T.-T. Yip, L. Lomas, et al., "Classification of cancer types by measuring variants of host response proteins using SELDI serum assays," *International Journal of Cancer*, vol. 115, no. 5, pp. 783–789, 2005.
- [124] J. Peng, A. J. Stanley, D. Cairns, P. J. Selby, and R. E. Banks, "Using the protein chip interface with quadrupole time-of-flight mass spectrometry to directly identify peaks in SELDI profiles—initial evaluation using low molecular weight serum peaks," *Proteomics*, vol. 9, no. 2, pp. 492–498, 2009.
- [125] R. N. H. Pugh, I. M. Murray Lyon, J. L. Dawson, M. C. Pietroni, and R. Williams, "Transection of the oesophagus for bleeding oesophageal varices," *British Journal of Surgery*, vol. 60, no. 8, pp. 646–649, 1973.
- [126] L. Brugler, A. Stankovic, L. Bernstein, F. Scott, and J. O'Sullivan-Maillet, "The role of visceral protein markers in protein calorie malnutrition," *Clinical Chemistry and Laboratory Medicine*, vol. 40, no. 12, pp. 1360–1369, 2002.
- [127] P. B. Sehgal, "Interleukin-6: molecular pathophysiology," *Journal of Investigative Dermatology*, vol. 94, no. 6, supplement, pp. 2S–6S, 1990.
- [128] E. P. Diamandis, "Point: proteomic patterns in biological fluids: do they represent the future of cancer diagnostics?" *Clinical Chemistry*, vol. 49, no. 8, pp. 1272–1275, 2003.
- [129] N. Escher, M. Kaatz, C. Melle, et al., "Posttranslational modifications of transthyretin are serum markers in patients with mycosis fungoides," *Neoplasia*, vol. 9, no. 3, pp. 254–259, 2007.
- [130] M. Ueda, Y. Misumi, M. Mizuguchi, et al., "SELDI-TOF mass spectrometry evaluation of variant transthyretins for diagnosis and pathogenesis of familial amyloidotic polyneuropathy," *Clinical Chemistry*, vol. 55, no. 6, pp. 1223–1227, 2009.
- [131] L. Chen, S. Fatima, J. Peng, and X. Leng, "SELDI protein chip technology for the detection of serum biomarkers for liver disease," *Protein and Peptide Letters*, vol. 16, no. 5, pp. 467–472, 2009.
- [132] B. Matharoo-Ball, G. Ball, and R. Rees, "Clinical proteomics: discovery of cancer biomarkers using mass spectrometry and bioinformatics approaches—a prostate cancer perspective," *Vaccine*, vol. 25, supplement 2, pp. B110–B121, 2007.
- [133] A. Skytt, E. Thysell, P. Stattin, et al., "SELDI-TOF MS versus prostate specific antigen analysis of prospective plasma samples in a nested case-control study of prostate cancer," *International Journal of Cancer*, vol. 121, no. 3, pp. 615–620, 2007.
- [134] G. Xu, C. Q. Xiang, Y. Lu, et al., "Application of SELDI-TOF-MS to identify serum biomarkers for renal cell carcinoma," *Cancer Letters*, vol. 282, no. 2, pp. 205–213, 2009.
- [135] B. J. McMorran, S. A. O. Patat, J. B. Carlin, et al., "Novel neutrophil-derived proteins in bronchoalveolar lavage fluid indicate an exaggerated inflammatory response in pediatric cystic fibrosis patients," *Clinical Chemistry*, vol. 53, no. 10, pp. 1782–1791, 2007.
- [136] C. Rocken, R. Ketterlinus, and M. P. A. Ebert, "Application of proteome analysis to the assessment of prognosis and

response prediction in clinical oncology,” *Current Cancer Drug Targets*, vol. 8, no. 2, pp. 141–145, 2008.

- [137] C. Trocme, H. Marotte, A. Baillet, et al., “Apolipoprotein A-I and platelet factor 4 are biomarkers for infliximab response in rheumatoid arthritis,” *Annals of the Rheumatic Diseases*, vol. 68, no. 8, pp. 1328–1333, 2009.